Flow	± (2 L/min + 10 % of the actual reading) (BTPS)
Log	
Type	Alarm, Operation
Max number	5000
O_2 Sensor	
Type	Galvanic fuel cell
Response time	< 15 s
Communication interface	
Communication interface	Rs232, Ethernet, VGA, USB port, Nurse call
Gas supply	
Gas type	O_2
Pipe Connector	NIST or DISS
Gas supply pressure	280 - 600 kPa
Peak flow in case of single supply gas(air)	≥ 210 L/min (BTPS)*[1]
Operation Data	
Environmental specifications	
Temperature	5 - 40 °C (operating); -20 to 60 °C (storage and transport, O_2 sensor: -20 to 50°C)
Relative Humidity	10 - 95 % (operating); 10 - 95 % (storage and transport)
Barometric Pressure	62 - 106 kPa (operating); 50 -106 kPa (storage and transport)
Power and Battery Backup	
External AC power supply	
Input voltage	100 - 240 V
Input frequency	50/60 Hz
Input current	2.7 - 1.1 A
Fuse	T3.15 AH/250 V
External DC power supply	
Input voltage	12 V
Input current	15 A
Internal battery	
Number of batteries	One or Two
Battery type	Build-in Lithium-ion battery, 14.8 VDC, 5800 mAh
Battery run time	180 min (Powered by one new fully - charged battery in standard working condition)*[2] 360 min (Powered by two new fully - charged battery in standard working condition)
Trolley	
Dimensions	1039 mm*528 mm*544 mm
Weight	Approximately 20 kg
Special Functions and procedures	
Sigh	
100% O_2	
Suction	
Manual breath	
Expiratory hold	
Inspiratory hold	
P0.1	
NIF	
PV - Tool	
PEEPi	
Nebulizer	
O_2 Therapy	

*[1] *BTPS =Body Temperature and Pressure Saturated*
*[2] *The standard work condition is:Ventilation mode:P-A/C ; ΔPinsp:10 cmH_2O; f:10 bpm; Tinsp:2 s ; Tslope:0.2 s ; O_2%:21 Vol.%; PEEP:5 cmH_2O ; R:20 cmH_2O/L/s ; C:20 ml/cmH_2O ; Gas supply nominal work pressure:400±100 kPa.*

The materials and information provided via this brochure are distributed internationally, but not all the products or services found on this brochure are necessarily available in your country or area. Please contact local office or agents to make sure of the availability of the relevant products or services.

Mindray Medical Netherlands B.V.
Drs.W.van Royenstraat 8, 3871 AN Hoevelaken, The Netherlands
Voice: (31-33) 254-4911
Fax: (31-33) 253-4280

Mindray Medical Italy S.r.l.
Via Leonardo DA Vinci, 15B, 20090 Trezzano Sul Naviglio (MI), Italy
Voice: (39-02) 5737-401
Fax: (39-02) 5523-2018

Mindray Medical España S.L.
Avenida Manoteras 38, Edificio B, Bajo B008. 28050-Madrid Spain
Voice: (34-91) 392-3754
Fax: (34-91) 392-3756

Mindray Medical Germany GmbH
Goebelstrasse 21, 3. OG, 64293 Darmstadt
Voice: (49 6151) 3910 0
Fax: (49 6151) 3910 300

Mindray (UK) Limited
Mindray House, Kingfisher Way, Hinchingbrooke Business Park, Huntingdon, Cambs, PE29 6FN
Voice: (44) 1480-416-840
Fax: (44) 1480-436-588

Mindray Medical France SARL
Europarc Creteil 1 allée des cerisiers 94000 CRETEIL, France
Voice: (33-1) 4513-9150
Fax: (33-1) 4513-9151

Mindray Medical Sweden AB
Rissneleden 136, 174 57 Sundbyberg, Sweden
Voice: (46) 8 555 54 121

Mindray Medical Rus Co.Ltd
2 Zvenigorodskaya Street, 13, bld 41, 123022 Moscow, Russia
Voice: (7-499) 553-6036
Fax: (7-499) 553-6039

Mindray Medical Colombia S.A.S
Room No.702, Torre UNIKA,Carrera 9 No.77-67, Bogota, Colombia
Voice: (57-1) 3130892 / 3210916

Mindray do Brasil – Comércio e Distribuição de Equipamentos Médicos Ltda.
Rua Tavares Bastos, 329, Perdizes, São Paulo - SP.
CEP 05012-020
Voice: (55-11) 3124-8026
Fax: (55-11) 3078-8035

Mindray Medical Mexico S. de R.L. de C.V.
Félix Parra # 175 Colonia. San José Insurgentes Sur Delegación Benito Juárez 03900 México, D. F.
Voice: (52-55) 5661-9450 / (52-55) 5662-6620
Fax: (52-55) 5662-6597

PT.Mindray Medical Indonesia
The East 11th Floor, Unit 08 Jl. Dr. Ide Anak Agung Gde Agung Kav. E 3.2 No.1 Jakarta 12950
Voice: (6221) 2902-7280
Fax: (6221) 2902-7283

Mindray Medical Egypt
Ground Floor -11 El Imam Metwally El Sharawi Street, Sheraton Heliopolis - El Nozha, Cairo, Egypt
Voice: (2) 02 22691047
Fax: (2) 02 22691046

Mindray Medical Australia
ADD: 19 Harker St, Burwood VIC 3125, Australia
Voice: (61-3) 9830 6610
Fax: (61-2) 9550 2841

Mindray Medical Nigeria
ADD: 1004 Estate,Victoria Island, Lagos, Nigeria
Voice: (+234) 7030682053

Mindray Medical India Pvt. Ltd. (Delhi Office)
16th floor, Building No. 9-B, DLF Cyber City, DLF Phase- 3, Gurgaon- 122002, Haryana
Voice: (91-124) 4632-488
Fax: (91-124) 4632499

Mindray Medical India Pvt. Ltd. (Mumbai office)
B-404, City Point, Andheri Kurla Road, Andheri East, Mumbai, 400 059, India
Voice: (91-22) 4020-0000
Fax: (91-22) 4020-0011


Mindray Medikal Teknoloji Istanbul Ltd. Sti.
KÖYALTI MEVKİİ 29 EKİM CAD.N.1 KUYUMCUKENT 2.NO.PLZ.3.KT. D.1- 9 34520 BAHÇELİEVLER/YENİBOSNA, ISTANBUL, TÜRKİYE
Voice: (90-212) 482 08 77
Fax: (90-212) 482 08 78

Mindray Medikal Teknoloji Istanbul Ltd. Sti. Branch Office Ankara
TURAN GÜNEŞ BULVARI ALEKSANDER DÜBÇEK CAD. NO:18/A
ÇANKAYA/ANKARA, TÜRKİYE
Voice: (90-312) 441 96 92
Fax: (90-312) 441 96 93

Mindray Medical Vietnam Co.,Ltd.
Unit 2, 4th Floor, "B" Building, Broadway Office Park, 102 Nguyen Luong Bang Blvd., Tan Phu Ward, Dist. 7, HCMC, Vietnam
Voice: (84) 8 5413-6970
Fax: (84) 8 5413-6971

Mindray Medical Thailand Limited
1768 Thai summit Tower Room 407, 4th floor, New petchaburee Road, Kwaeng Bangkapi, Khet Huai Khwang, Bangkok 10320, Thailand
Voice: (66) 2652-7288
Fax: (66) 2652-7266

Mindray Medical Korea
KNI Tower 9F 823-19 Yeoksam dong, Seoul-ganum, Korea
Tel: 008225688040
Fax: 008225688042

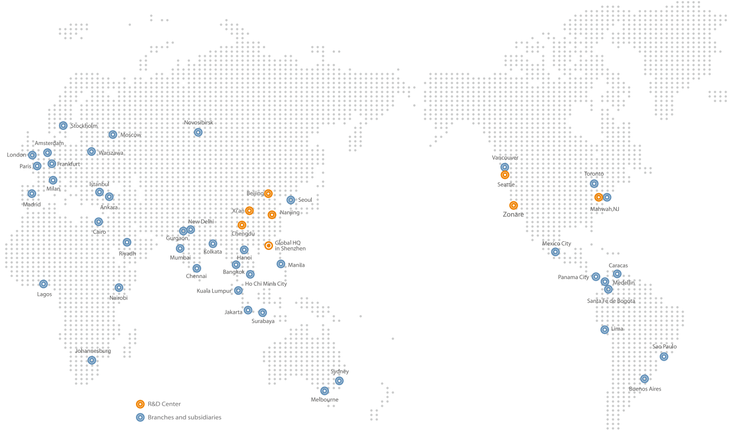

Mindray Building, Keji 12th Road South,
High-tech Industrial Park, Nanshan, Shenzhen 518057, P.R. China
Tel: +86 755 8188 8998 Fax: +86 755 26582680
E-mail: intl-market@mindray.com www.mindray.com

mindray | trademarks within each are registered trademarks or trademarks owned by Shenzhen Mindray Bio-medical Electronics Co., LTD.
©2015 Shenzhen Mindray Bio-Medical Electronics Co., Ltd. All rights reserved. Specifications subject to changes without prior notice.

P/N:ENG-SV 300 datasheet-210285x6P-20170317

mindray



SV300
Ventilator

Technical Specifications

Physical Specification	
Dimensions	354 mm*315 mm*249 mm (Excluding the trolley)
Weight	Approximately 10 kg (Excluding the trolley)
Screen	
Display Size	12.1 Color active matrix TFT touch
Display Resolution (H) x (V)	1280*800 pixels
Brightness	Adjustable
Ventilation Specifications	
Patient Type	Adults, children, infants (body weight of at least 3 kg)
Ventilation Mode	V-A/C (Volume assist/control) P-A/C (Pressure assist/control) V-SIMV (Volume - Synchronized Intermittent Mandatory Ventilation) P-SIMV (Pressure - Synchronized Intermittent Mandatory Ventilation) DuoLevel (Duo Level Ventilation) CPAP (Continuous Positive Airway Pressure) PSV (Pressure Support Ventilation) APRV (Airway Pressure Release Ventilation) PRVC (Pressure Regulated Volume Control) PRVC-SIMV ((Pressure Regulated Volume Control- Synchronized Intermittent Mandatory Ventilation) NIV (Non-invasive ventilation) Apnea Ventilation
Controlled Parameters	
O_2%	21 - 100% (increments of 1 %)
TV(Tidal Volume)	Adult: 100 - 2000 mL (increments of 10 mL) Pediatric: 20 - 300 mL (increments of 1 mL)
f (Ventilation frequency)	1 - 100 bpm (increments of 1 bpm)
fSIMV (Ventilation frequency in SIMV mode)	1 - 60 bpm (increments of 1 bpm)
I:E range	4:1 - 1:10 (increments of 0.5)
Tinsp (Inspiratory time)	0.20 - 10 s (increments of 0.05 s)
Tslope (Time of Pressure Rising)	0 - 2.00 s (increments of 0.05 s)
Thigh	0.2 - 30 s (increments of 0.1 s)
Tlow	0.2 - 30 s (increments of 0.1 s)
Tpause	5 % - 60 % (increments of 5 %), Off
ΔPinsp	5 - 80 cmH_2O (increments of 1 cmH_2O)
ΔPsupp	0 - 80 cmH_2O (increments of 1 cmH_2O)
Phigh	0 - 80 cmH_2O (increments of 1 cmH_2O)
Plow	0 - 45 cmH_2O (increments of 1 cmH_2O)
PEEP	1 - 45 cmH_2O (increments of 1 cmH_2O), Off
Flow trigger	0.5 -15 L/min (increments of 0.1 L/min), Off
Pressure trigger	-10 to - 0.5 cmH_2O (increments of 0.5 cmH_2O), Off
Exp % (Expiration termination level)	10 - 85% (increments of 5%), Auto
Apnea Ventilation	
Tvapnea	Adult: 100 - 2000 mL (increments of 10 mL) Pediatric: 20 - 300 mL (increments of 1 mL)
ΔPapnea	5 - 80 cmH_2O (increments of 1 cmH_2O)
fapnea	1 - 80 bpm (increments of 1 bpm)
Apnea Tinsp	0.20 - 10 s (increments of 0.05 s)

Sigh	
Sigh Switch	ON, Off
Interval	20 s - 180 min (increments of 1 s from 20 to 59 s, increments of 1 min from 1 to 180 min)
Cycles Sigh	1 - 20 (increments of 1)
ΔinT.PEEP	1 - 45 cmH_2O (increments of 1 cmH_2O), Off
Automatic Tube Resistance Compensation	
Tube Type	ET Tube, Trach Tube, Disable ATRC
Tube I.D.	Adult: 5.0 - 12.0 mm (increments of 0.5 mm) Pediatric: 2.5 - 8.0 mm (increments of 0.5 mm)
Compensate	0 -100 % (increments of 1 %)
Expiration Compensation Switch	ON, Off
Monitored parameters	
Airway pressure range	Ppeak, Pplat, Pmean, PEEP (Range 0 - 120 cmH_2O)
Tidal volume range	TVi, TVe, TVe spn (Range 0 - 4000 mL)
Frequency range	ftotal, fmand, fspn (Range 0 - 200 bpm)
Minute volume range	MV, MVspn, MVleak (Range 0 - 100 L/min)
Resistance	Rinsp, Rexp (0 - 600 cmH_2O/L/s)
Compliance	Cstat, Cdyn (0 - 300 mL/cmH_2O)
Inspired Oxygen(FiO_2)	15 - 100 %
RSBI	0 - 999 1/(L•min)
WOB	0 - 100 J/min
P0.1	-20 - 0 cmH_2O
NIF	-45 - 0 cmH_2O
PEEPi	0 - 80 cmH_2O
RCexp	0 - 10 s
TVe/IBW	0 - 50 ml/kg
I:E	100:1 -1:150
Tinsp	0.00 - 60.00s
Waveforms	Airway pressure - time, Flow - time, Volume - time
Loops	Paw - Volume, Flow - Volume, Paw - Flow
Ventilator Accuracy	
Control Accuracy	
O_2 %	± (3 vol.% +1 % of setting)
TV	± (10 mL + 10 % of setting) (BTPS)
Tinsp	± 0.1 s or ± 10 % of setting, whichever is greater
I: E	2: 1 to 1: 4: ± 10 % of setting, other range: ± 15% of setting
f	± 1 bpm
fSIMV	± 1 bpm
Tslope	± (0.2 s + 20 % of setting)
PEEP	± (2.0 cmH_2O + 5 % of setting)
ΔPinsp	± (2.0 cmH_2O + 5 % of setting)
ΔPsupp	± (2.0 cmH_2O + 5 % of setting)
Phigh	± (2.0 cmH_2O + 5 % of setting)
Plow	± (2.0 cmH_2O + 5 % of setting)
Thigh	± 0.2 s or ± 10 % of setting, whichever is greater
Tlow	± 0.2 s or ± 10 % of setting, whichever is greater
Pressure Trigger	± (1.0 cmH_2O + 10 % of setting)
Flow Trigger	± (1.0 L/min + 10 % of setting)
ΔinT.PEEP	± (2.0 cmH_2O + 5% of setting)
Exp %	± 10 %
fapnea	± 1 bpm
ΔPapnea	± (2.0 cmH_2O + 5 % of setting)
TVapnea	± (10 mL + 10 % of setting) (BTPS)
Apnea Tinsp	± 0.1 s or ± 10% of setting, whichever is greater

Monitoring Accuracy		
Airway pressure (Ppeak, Pplat, Pmean, PEEP)		± (2 cmH_2O + 4 % of the actual reading)
Tidal Volume (TVi, TVe, TVe/IBW, TVe spn)		0 ml - 100 ml: ± (10 ml + 3 % of the actual reading) (BTPS); 100 ml - 4000 ml: ± (3 ml + 10 % of the actual reading) (BTPS)
Minute Volume (MV, MVspn, MVleak)		± (0.2 L/min + 10 % of the actual reading) (BTPS)
Frequency (ftotal, fmand, fspn)		± 5% of reading or ± 1bpm, whichever is greater
Inspired Oxygen (FiO_2)		± (2.5 vol.% + 2.5 % of the actual reading)
Resistance		0 to 20: ± 10 cmH_2O/L/s Other range: 50 % of actual reading
Compliance		± (2 ml/cmH_2O + 20 % of the actual reading)
RSBI		± (3 1/(L•min)+15 % of the actual reading)
WOB		± (1 J/min+15 % of the actual reading)
NIF		± (2 cmH_2O + 4 % of the actual reading)
P0.1		± (2 cmH_2O + 4 % of the actual reading)
PEEPi		No declaration
RCexp		± (0.2 s + 20 % of the actual reading)
Alarm settings		
Tidal Volume	High	Adult: 110 - 4000 mL, Off Pediatric: 25 - 600 mL, Off
	Low	Adult: 50 - 4000 ml, Off Pediatric: 10 - 600 mL, Off
Minute Volume	High	Adult: 0.2 - 100.0 L/min Pediatric: 0.2 - 60.0 L/min
	Low	Adult: 0.1 - 50.0 L/min Pediatric: 0.1 - 30.0 L/min
Air pressure	High	10 - 85 cmH_2O
Frequency	High	1 - 150 bpm, Off
Inspired oxygen (FiO_2)	High	Auto, FiO_2 exceeds the alarm limit for at least 30 s, internal alarm limit: min (set value+max (7 % or set value*10 %), 100 %)
	Low	Auto, FiO_2 lower than the alarm limit for at least 30 s, internal alarm limit: max (set value-max (7 % or set value*10 %),18 %), Absolute FiO_2 low limit: 18 %
Apnea alarm time		5 - 60 s
SideStream CO_2 Module (optional)		
Displayed numerics		$EtCO_2$
Measurement Range		0 - 99 mmHg
Measurement accuracy		0 to 40 mmHg ± 2 mmHg 41 to 76 mmHg ± 5% of reading 77 to 99 mmHg ± 10% of reading
Waveforms		$EtCO_2$ - time
Resolution		1 mmHg
Sampling rate		Adult: 70 ml/min, 100 ml/min, 120 ml/min, 150 ml/min Pediatric: 70 ml/min, 100 ml/min
Sampling rate Accuracy		± 15% of the set value or ± 15 mL/min, whichever is greater
System response time		Using Adult water trap, Adult sampling line: < 7.5 s @ 150 ml/min < 8.0 s @ 120 ml/min < 8.5 s @ 100 ml/min < 9.5 s @ 70 ml/min Using Pediatric water trap, Pediatric sampling line: < 7.5 s @ 100 ml/min < 8.0 s @ 70 ml/min
Rise time		Adult water trap: < 400 ms @70 ml/min < 330 ms @100 ml/min < 300 ms @120 ml/min < 240 ms @150 ml/min Pediatric water trap: < 400 ms @70 ml/min < 330 ms @100 ml/min
Water trap cleaning time		Adult water trap: ≥24 h @150 ml/min ≥48 h @70 ml/min Pediatric water trap: ≥24 h @100 ml/min ≥48 h @70 ml/min

Sidestream CO_2 alarm limits		
$EtCO_2$	High	2 - 99 mmHg
	Low	0 - 97 mmHg
MainStream CO_2 Module(optional)		
Displayed numerics		$EtCO_2$
$EtCO_2$ Measurement range		0 -150 mmHg
$EtCO_2$ Measurement Accuracy		0 to 40 mmHg ± 2 mmHg of reading 41 to 70 mmHg ± 5% of reading 71 to 100 mmHg ± 8% of reading 101 to 150 mmHg ± 10% of reading
Resolution		1 mmHg
Waveforms		$EtCO_2$ - time, Volume - $EtCO_2$
Other Parameters		
$SlopeCO_2$ (slope of the alveolar plateau)		Range: 0 - 9.99 %/L Resolution: 0.01 %/L
Vtalv (Alveolar tidal ventilation)		Range: 0 - 9999 ml Resolution: 1 ml
V'alv (Alveolar minute ventilation)		Range: 0 - 20 L/min Resolution: 0.01 L/min for < 1 L/min, 0.1 L/min for ≥ 1 L/min
$V'CO_2$ (CO_2 elimination)		Range: 0 - 9999 mL/min Resolution: 1 ml/min
VDaw (Airway death space)		Range: 0 - 999 mL Resolution: 1 ml
VDaw/TVe (Physiological dead space fraction at the airway opening)		Range: 0 - 100 % Resolution: 1 %
$VeCO_2$ (exhaled CO_2 volume)		Range: 0 - 999 mL Resolution: 1 ml
$ViCO_2$ (inspired CO_2 volume)		Range: 0 - 999 mL Resolution: 1 ml
System response time		< 2.0 s
CO_2 alarm limits		
$EtCO_2$	High	2 - 150 mmHg
	Low	0 - 148 mmHg
SpO_2 module(optional)		
Measurement Range and Resolution		
SpO_2		Range: 0 - 100 % Resolution: 1 %
PR		Range: 20 - 254 1/min Resolution: 1 1/min
PI		Range: 0.05 - 20 %
Measurement Accuracy		
SpO_2		70 to 100 %: ±2 % 0 % to 69 %: Not specified.
PR		± 3 1/min
SpO_2 alarm limits		
SpO_2	High	2 -100 %
	Low	0 - 98 %
	Desat	0 - 98 %
PR	High	17 - 300 1/min
	Low	15 - 298 1/min
Trend		
Type		Tabular, Graphic
Length		72 hours
Content		Monitor Parameters, Setting Parameters (Setting Ventilation mode and Parameters)
O_2 Therapy		
Controlled Parameters		
O_2 %		21 - 100 % (increments of 1 %)
Flow		2 - 60 L/min
Controlled Accuracy		
O_2 %		± (3 vol.% +1 % of setting)
Flow		± (2 L/min +10 % of setting) (BTPS)
Monitor Accuracy		
FiO_2		± (2.5 vol. % + 2.5 % of the actual reading)