Boston Scientific

**2.0mm x 9mm**

# Maverick²™

## MONORAIL™


### PTCA Dilatation Catheter

Catéter de dilatación para ACTP, Cathéter de dilatation pour ACTP, PTCA-Dilatationskatheter, Catetere dilatatore per PTCA, PTCA dilatatiekatheter, PTCA拡張カテーテル, PTCA-dilatationskateter, Καθετήρας διαστολής PTCA, Cateter de Dilatação para PTCA, PTCA-dilatationskateter, PTCA-tágítókatéter, Dilatační katétr pro PTCA, Cewnik rozszerzający do PTCA, PTCA-dilatasjonskateter, PTKA Dilatasyon Kateteri

| atm - kPa Pressure | | 2.0mm Balloon O.D. |
|---|---|---|
| 5.0 - 507 | | 1.97 |
| 6.0 - 608 | NOMINAL | 2.00 |
| 7.0 - 709 | | 2.03 |
| 8.0 - 811 | | 2.06 |
| 9.0 - 912 | | 2.09 |
| 10.0 - 1013 | | 2.12 |
| 11.0 - 1115 | | 2.15 |
| 12.0 - 1216 | RATED* | 2.19 |
| 13.0 - 1317 | | -- |
| 14.0 - 1419 | | -- |

*Rated Burst Pressure. DO NOT EXCEED.

Contents (1)




CL (1) Includes CLIPIT™ Hypotube Clip

GW R 0.014in (≤0.36mm) Recommended Guidewire

GC R 5F (≥0.058in/1.47mm) Recommended Guide Catheter

| | | | |
|---|---|---|---|
| **GTIN** | 08714729369875 | LOT | 12345678 |
| REF Catalog No. | H749389280920 0 | Use By | 2010-12-31 |

STERILE EO Sterilized using ethylene oxide.

90244533-01

Internal BSC Bar Code

92425134-01A

CE 0344

**Made in MALAYSIA**
PMT 741, Persiaran Cassia Selatan 1
Taman Perindustrian Batu Kawan
14110 Bandar Cassia,
Pulau Pinang, MALAYSIA

Boston Scientific
Maverick²™
2.0mm x 9mm
GTIN 08714729369875
REF H7493892809200
LOT 12345678

Boston Scientific
Maverick²™
2.0mm x 9mm
GTIN 08714729369875
REF H7493892809200
LOT 12345678

(01)08714729369875(17)101231(10)12345678 GS1

This product may be protected by one or more patents. Patent information can be obtained at http://www.bostonscientific.com/patents

**Label Specification Part Number:92425134-01A**

Boston Scientific

**2.25mm x 9mm**

# Maverick²™

## MONORAIL™


### PTCA Dilatation Catheter

Catéter de dilatación para ACTP, Cathéter de dilatation pour ACTP, PTCA-Dilatationskatheter, Catetere dilatatore per PTCA, PTCA dilatatiekatheter, PTCA拡張カテーテル, PTCA-dilatationskateter, Καθετήρας διαστολής PTCA, Cateter de Dilatação para PTCA, PTCA-dilatationskateter, PTCA-tágítókatéter, Dilatační katétr pro PTCA, Cewnik rozszerzający do PTCA, PTCA-dilatasjonskateter, PTKA Dilatasyon Kateteri

| atm - kPa Pressure | | 2.25mm Balloon O.D. |
|---|---|---|
| 5.0 - 507 | | 2.22 |
| 6.0 - 608 | NOMINAL | 2.25 |
| 7.0 - 709 | | 2.28 |
| 8.0 - 811 | | 2.31 |
| 9.0 - 912 | | 2.35 |
| 10.0 - 1013 | | 2.38 |
| 11.0 - 1115 | | 2.41 |
| 12.0 - 1216 | | 2.44 |
| 13.0 - 1317 | | 2.47 |
| 14.0 - 1419 | RATED* | 2.51 |

*Rated Burst Pressure and Stent Rated Burst Pressure. DO NOT EXCEED.

Contents (1)




CL (1) Includes CLIPIT™ Hypotube Clip

GW R 0.014in (≤0.36mm) Recommended Guidewire

GC R 5F (≥0.058in/1.47mm) Recommended Guide Catheter

| | | | |
|---|---|---|---|
| **GTIN** | 08714729369882 | LOT | 12345678 |
| REF Catalog No. | H7493892809220 | Use By | 2010-12-31 |

STERILE EO Sterilized using ethylene oxide.

90244533-01

Internal BSC Bar Code

92425134-02A

CE 0344

**Made in MALAYSIA**
PMT 741, Persiaran Cassia Selatan 1
Taman Perindustrian Batu Kawan
14110 Bandar Cassia,
Pulau Pinang, MALAYSIA

Boston Scientific
Maverick²™
2.25mm x 9mm
GTIN 08714729369882
REF H7493892809220
LOT 12345678

Boston Scientific
Maverick²™
2.25mm x 9mm
GTIN 08714729369882
REF H7493892809220
LOT 12345678

(01)08714729369882(17)101231(10)12345678 GS1

This product may be protected by one or more patents. Patent information can be obtained at http://www.bostonscientific.com/patents

**Label Specification Part Number:92425134-02A**

Boston Scientific

**2.5mm x 9mm**

# Maverick²™

## MONORAIL™


### PTCA Dilatation Catheter

Catéter de dilatación para ACTP, Cathéter de dilatation pour ACTP, PTCA-Dilatationskatheter, Catetere dilatatore per PTCA, PTCA dilatatiekatheter, PTCA拡張カテーテル, PTCA-dilatationskateter, Καθετήρας διαστολής PTCA, Cateter de Dilatação para PTCA, PTCA-dilatationskateter, PTCA-tágítókatéter, Dilatační katétr pro PTCA, Cewnik rozszerzający do PTCA, PTCA-dilatasjonskateter, PTKA Dilatasyon Kateteri

| atm - kPa Pressure | | 2.5mm Balloon O.D. |
|---|---|---|
| 5.0 - 507 | | 2.46 |
| 6.0 - 608 | NOMINAL | 2.50 |
| 7.0 - 709 | | 2.54 |
| 8.0 - 811 | | 2.58 |
| 9.0 - 912 | | 2.62 |
| 10.0 - 1013 | | 2.67 |
| 11.0 - 1115 | | 2.71 |
| 12.0 - 1216 | | 2.75 |
| 13.0 - 1317 | | 2.79 |
| 14.0 - 1419 | RATED* | 2.83 |

*Rated Burst Pressure and Stent Rated Burst Pressure. DO NOT EXCEED.

Contents (1)




CL (1) Includes CLIPIT™ Hypotube Clip

GW R 0.014in (≤0.36mm) Recommended Guidewire

GC R 5F (≥0.058in/1.47mm) Recommended Guide Catheter

| | | | |
|---|---|---|---|
| **GTIN** | 08714729369899 | LOT | 12345678 |
| REF Catalog No. | H749389280925 0 | Use By | 2010-12-31 |

STERILE EO Sterilized using ethylene oxide.

90244533-01

Internal BSC Bar Code

92425134-03A

CE 0344

**Made in MALAYSIA**
PMT 741, Persiaran Cassia Selatan 1
Taman Perindustrian Batu Kawan
14110 Bandar Cassia,
Pulau Pinang, MALAYSIA

Boston Scientific
Maverick²™
2.5mm x 9mm
GTIN 08714729369899
REF H7493892809250
LOT 12345678

Boston Scientific
Maverick²™
2.5mm x 9mm
GTIN 08714729369899
REF H7493892809250
LOT 12345678

(01)08714729369899(17)101231(10)12345678 GS1

This product may be protected by one or more patents. Patent information can be obtained at http://www.bostonscientific.com/patents

**Label Specification Part Number:92425134-03A**

Boston Scientific

**2.75mm x 9mm**

# Maverick²™

## MONORAIL™


### PTCA Dilatation Catheter

Catéter de dilatación para ACTP, Cathéter de dilatation pour ACTP, PTCA-Dilatationskatheter, Catetere dilatatore per PTCA, PTCA dilatatiekatheter, PTCA拡張カテーテル, PTCA-dilatationskateter, Καθετήρας διαστολής PTCA, Cateter de Dilatação para PTCA, PTCA-dilatationskateter, PTCA-tágítókatéter, Dilatační katétr pro PTCA, Cewnik rozszerzający do PTCA, PTCA-dilatasjonskateter, PTKA Dilatasyon Kateteri

| atm - kPa Pressure | | 2.75mm Balloon O.D. |
|---|---|---|
| 5.0 - 507 | | 2.71 |
| 6.0 - 608 | NOMINAL | 2.75 |
| 7.0 - 709 | | 2.79 |
| 8.0 - 811 | | 2.83 |
| 9.0 - 912 | | 2.87 |
| 10.0 - 1013 | | 2.91 |
| 11.0 - 1115 | | 2.95 |
| 12.0 - 1216 | | 2.99 |
| 13.0 - 1317 | | 3.03 |
| 14.0 - 1419 | RATED* | 3.07 |

*Rated Burst Pressure and Stent Rated Burst Pressure. DO NOT EXCEED.

Contents (1)




CL (1) Includes CLIPIT™ Hypotube Clip

GW R 0.014in (≤0.36mm) Recommended Guidewire

GC R 5F (≥0.058in/1.47mm) Recommended Guide Catheter

| | | | |
|---|---|---|---|
| **GTIN** | 08714729369905 | LOT | 12345678 |
| REF Catalog No. | H749389280927o | Use By | 2010-12-31 |

STERILE EO Sterilized using ethylene oxide.

90244533-01

Internal BSC Bar Code

92425134-04A

CE 0344

**Made in MALAYSIA**
PMT 741, Persiaran Cassia Selatan 1
Taman Perindustrian Batu Kawan
14110 Bandar Cassia,
Pulau Pinang, MALAYSIA

Boston Scientific
Maverick²™
2.75mm x 9mm
GTIN 08714729369905
REF H7493892809270
LOT 12345678

Boston Scientific
Maverick²™
2.75mm x 9mm
GTIN 08714729369905
REF H7493892809270
LOT 12345678

(01)08714729369905(17)101231(10)12345678 GS1

This product may be protected by one or more patents. Patent information can be obtained at http://www.bostonscientific.com/patents

**Label Specification Part Number:92425134-04A**

Boston Scientific

**3.0mm x 9mm**

# Maverick²™

## MONORAIL™


### PTCA Dilatation Catheter

Catéter de dilatación para ACTP, Cathéter de dilatation pour ACTP, PTCA-Dilatationskatheter, Catetere dilatatore per PTCA, PTCA dilatatiekatheter, PTCA拡張カテーテル, PTCA-dilatationskateter, Καθετήρας διαστολής PTCA, Cateter de Dilatação para PTCA, PTCA-dilatationskateter, PTCA-tágítókatéter, Dilatační katétr pro PTCA, Cewnik rozszerzający do PTCA, PTCA-dilatasjonskateter, PTKA Dilatasyon Kateteri

| atm - kPa Pressure | | 3.0mm Balloon O.D. |
|---|---|---|
| 5.0 - 507 | | 2.95 |
| 6.0 - 608 | NOMINAL | 3.00 |
| 7.0 - 709 | | 3.05 |
| 8.0 - 811 | | 3.09 |
| 9.0 - 912 | | 3.14 |
| 10.0 - 1013 | | 3.18 |
| 11.0 - 1115 | | 3.23 |
| 12.0 - 1216 | | 3.28 |
| 13.0 - 1317 | | 3.32 |
| 14.0 - 1419 | RATED* | 3.37 |

*Rated Burst Pressure and Stent Rated Burst Pressure. DO NOT EXCEED.

Contents (1)




CL (1) Includes CLIPIT™ Hypotube Clip

GW R 0.014in (≤0.36mm) Recommended Guidewire

GC R 5F (≥0.058in/1.47mm) Recommended Guide Catheter

| | | | |
|---|---|---|---|
| **GTIN** | 08714729369912 | LOT | 12345678 |
| REF Catalog No. | H749389280930o | Use By | 2010-12-31 |

STERILE EO Sterilized using ethylene oxide.

90244533-01

Internal BSC Bar Code

92425134-05A

CE 0344

**Made in MALAYSIA**
PMT 741, Persiaran Cassia Selatan 1
Taman Perindustrian Batu Kawan
14110 Bandar Cassia,
Pulau Pinang, MALAYSIA

Boston Scientific
Maverick²™
3.0mm x 9mm
GTIN 08714729369912
REF H7493892809300
LOT 12345678

Boston Scientific
Maverick²™
3.0mm x 9mm
GTIN 08714729369912
REF H7493892809300
LOT 12345678

(01)08714729369912(17)101231(10)12345678 GS1

This product may be protected by one or more patents. Patent information can be obtained at http://www.bostonscientific.com/patents

**Label Specification Part Number:92425134-05A**

Boston Scientific

**3.25mm x 9mm**

# Maverick²™

## MONORAIL™


### PTCA Dilatation Catheter

Catéter de dilatación para ACTP, Cathéter de dilatation pour ACTP, PTCA-Dilatationskatheter, Catetere dilatatore per PTCA, PTCA dilatatiekatheter, PTCA拡張カテーテル, PTCA-dilatationskateter, Καθετήρας διαστολής PTCA, Cateter de Dilatação para PTCA, PTCA-dilatationskateter, PTCA-tágítókatéter, Dilatační katétr pro PTCA, Cewnik rozszerzający do PTCA, PTCA-dilatasjonskateter, PTKA Dilatasyon Kateteri

| atm - kPa Pressure | | 3.25mm Balloon O.D. |
|---|---|---|
| 5.0 - 507 | | 3.20 |
| 6.0 - 608 | NOMINAL | 3.25 |
| 7.0 - 709 | | 3.30 |
| 8.0 - 811 | | 3.34 |
| 9.0 - 912 | | 3.39 |
| 10.0 - 1013 | | 3.43 |
| 11.0 - 1115 | | 3.48 |
| 12.0 - 1216 | | 3.52 |
| 13.0 - 1317 | | 3.57 |
| 14.0 - 1419 | RATED* | 3.61 |

*Rated Burst Pressure and Stent Rated Burst Pressure. DO NOT EXCEED.

Contents (1)




CL (1) Includes CLIPIT™ Hypotube Clip

GW R 0.014in (≤0.36mm) Recommended Guidewire

GC R 5F (≥0.058in/1.47mm) Recommended Guide Catheter

| | | | |
|---|---|---|---|
| **GTIN** | 08714729369929 | LOT | 12345678 |
| REF Catalog No. | H749389280932o | Use By | 2010-12-31 |

STERILE EO Sterilized using ethylene oxide.

90244533-01

Internal BSC Bar Code

92425134-06A

CE 0344

**Made in MALAYSIA**
PMT 741, Persiaran Cassia Selatan 1
Taman Perindustrian Batu Kawan
14110 Bandar Cassia,
Pulau Pinang, MALAYSIA

Boston Scientific
Maverick²™
3.25mm x 9mm
GTIN 08714729369929
REF H7493892809320
LOT 12345678

Boston Scientific
Maverick²™
3.25mm x 9mm
GTIN 08714729369929
REF H7493892809320
LOT 12345678

(01)08714729369929(17)101231(10)12345678 GS1

This product may be protected by one or more patents. Patent information can be obtained at http://www.bostonscientific.com/patents

**Label Specification Part Number:92425134-06A**

Boston Scientific

3.5mm x 9mm

# Maverick²™

## MONORAIL™


### PTCA Dilatation Catheter

Catéter de dilatación para ACTP, Cathéter de dilatation pour ACTP, PTCA-Dilatationskatheter, Catetere dilatatore per PTCA, PTCA dilatatiekatheter, PTCA拡張カテーテル, PTCA-dilatationskateter, Καθετήρας διαστολής PTCA, Cateter de Dilatação para PTCA, PTCA-dilatationskateter, PTCA-tágítókatéter, Dilatační katétr pro PTCA, Cewnik rozszerzający do PTCA, PTCA-dilatasjonskateter, PTKA Dilatasyon Kateteri

| atm - kPa Pressure | | 3.5mm Balloon O.D. |
|---|---|---|
| 5.0 - 507 | | 3.45 |
| 6.0 - 608 | NOMINAL | 3.50 |
| 7.0 - 709 | | 3.55 |
| 8.0 - 811 | | 3.60 |
| 9.0 - 912 | | 3.65 |
| 10.0 - 1013 | | 3.71 |
| 11.0 - 1115 | | 3.76 |
| 12.0 - 1216 | RATED* | 3.81 |
| 13.0 - 1317 | | -- |
| 14.0 - 1419 | | -- |

*Rated Burst Pressure and Stent Rated Burst Pressure. DO NOT EXCEED.

Contents (1)




CL (1) Includes CLIPIT™ Hypotube Clip

GW R 0.014in (≤0.36mm) Recommended Guidewire

GC R 5F (≥0.058in/1.47mm) Recommended Guide Catheter

| | | | |
|---|---|---|---|
| **GTIN** | 08714729369936 | LOT | 12345678 |
| REF Catalog No. | H749389280935o | Use By | 2010-12-31 |

STERILE EO Sterilized using ethylene oxide.

90244533-01

Internal BSC Bar Code

92425134-07A

CE 0344

**Made in MALAYSIA**
PMT 741, Persiaran Cassia Selatan 1
Taman Perindustrian Batu Kawan
14110 Bandar Cassia,
Pulau Pinang, MALAYSIA

Boston Scientific
Maverick²™
3.5mm x 9mm
GTIN 08714729369936
REF H7493892809350
LOT 12345678

Boston Scientific
Maverick²™
3.5mm x 9mm
GTIN 08714729369936
REF H7493892809350
LOT 12345678

(01)08714729369936(17)101231(10)12345678 GS1

This product may be protected by one or more patents. Patent information can be obtained at http://www.bostonscientific.com/patents

**Label Specification Part Number:92425134-07A**

Boston Scientific

3.75mm x 9mm

# Maverick²™

## MONORAIL™


### PTCA Dilatation Catheter

Catéter de dilatación para ACTP, Cathéter de dilatation pour ACTP, PTCA-Dilatationskatheter, Catetere dilatatore per PTCA, PTCA dilatatiekatheter, PTCA拡張カテーテル, PTCA-dilatationskateter, Καθετήρας διαστολής PTCA, Cateter de Dilatação para PTCA, PTCA-dilatationskateter, PTCA-tágítókatéter, Dilatační katétr pro PTCA, Cewnik rozszerzający do PTCA, PTCA-dilatasjonskateter, PTKA Dilatasyon Kateteri

| atm - kPa Pressure | | 3.75mm Balloon O.D. |
|---|---|---|
| 5.0 - 507 | | 3.70 |
| 6.0 - 608 | NOMINAL | 3.75 |
| 7.0 - 709 | | 3.80 |
| 8.0 - 811 | | 3.85 |
| 9.0 - 912 | | 3.90 |
| 10.0 - 1013 | | 3.95 |
| 11.0 - 1115 | | 4.00 |
| 12.0 - 1216 | RATED* | 4.05 |
| 13.0 - 1317 | | -- |
| 14.0 - 1419 | | -- |

*Rated Burst Pressure and Stent Rated Burst Pressure. DO NOT EXCEED.

Contents (1)




CL (1) Includes CLIPIT™ Hypotube Clip

GW R 0.014in (≤0.36mm) Recommended Guidewire

GC R 5F (≥0.058in/1.47mm) Recommended Guide Catheter

| | | | |
|---|---|---|---|
| GTIN | 08714729369943 | LOT | 12345678 |
| REF Catalog No. | H749389280937o | Use By | 2010-12-31 |

STERILE EO Sterilized using ethylene oxide.

90244533-01

Internal BSC Bar Code

92425134-08A

CE 0344

**Made in MALAYSIA**
PMT 741, Persiaran Cassia Selatan 1
Taman Perindustrian Batu Kawan
14110 Bandar Cassia,
Pulau Pinang, MALAYSIA

Boston Scientific
Maverick²™
3.75mm x 9mm
GTIN 08714729369943
REF H7493892809370
LOT 12345678

Boston Scientific
Maverick²™
3.75mm x 9mm
GTIN 08714729369943
REF H7493892809370
LOT 12345678

(01)08714729369943(17)101231(10)12345678 GS1

This product may be protected by one or more patents. Patent information can be obtained at http://www.bostonscientific.com/patents

**Label Specification Part Number:92425134-08A**

Boston Scientific

**4.0mm x 9mm**

# Maverick²™

## MONORAIL™


### PTCA Dilatation Catheter

Catéter de dilatación para ACTP, Cathéter de dilatation pour ACTP, PTCA-Dilatationskatheter, Catetere dilatatore per PTCA, PTCA dilatatiekatheter, PTCA拡張カテーテル, PTCA-dilatationskateter, Καθετήρας διαστολής PTCA, Cateter de Dilatação para PTCA, PTCA-dilatationskateter, PTCA-tágítókatéter, Dilatační katétr pro PTCA, Cewnik rozszerzający do PTCA, PTCA-dilatasjonskateter, PTKA Dilatasyon Kateteri

| atm - kPa Pressure | | 4.0mm Balloon O.D. |
|---|---|---|
| 5.0 - 507 | | 3.95 |
| 6.0 - 608 | NOMINAL | 4.00 |
| 7.0 - 709 | | 4.05 |
| 8.0 - 811 | | 4.10 |
| 9.0 - 912 | | 4.15 |
| 10.0 - 1013 | | 4.20 |
| 11.0 - 1115 | | 4.25 |
| 12.0 - 1216 | RATED* | 4.31 |
| 13.0 - 1317 | | -- |
| 14.0 - 1419 | | -- |

*Rated Burst Pressure and Stent Rated Burst Pressure. DO NOT EXCEED.

Contents (1)




CL (1) Includes CLIPIT™ Hypotube Clip

GW R 0.014in (≤0.36mm) Recommended Guidewire

GC R 5F (≥0.058in/1.47mm) Recommended Guide Catheter

| | | | |
|---|---|---|---|
| **GTIN** | 08714729369950 | LOT | 12345678 |
| REF Catalog No. | H749389280940o | Use By | 2010-12-31 |

STERILE EO Sterilized using ethylene oxide.

90244533-01

Internal BSC Bar Code

92425134-09A

CE 0344

**Made in MALAYSIA**
PMT 741, Persiaran Cassia Selatan 1
Taman Perindustrian Batu Kawan
14110 Bandar Cassia,
Pulau Pinang, MALAYSIA

Boston Scientific
Maverick²™
4.0mm x 9mm
GTIN 08714729369950
REF H7493892809400
LOT 12345678

Boston Scientific
Maverick²™
4.0mm x 9mm
GTIN 08714729369950
REF H7493892809400
LOT 12345678

(01)08714729369950(17)101231(10)12345678 GS1

This product may be protected by one or more patents. Patent information can be obtained at http://www.bostonscientific.com/patents

**Label Specification Part Number:92425134-09A**

Boston Scientific

**2.0mm x 12mm**

# Maverick²™

## MONORAIL™


### PTCA Dilatation Catheter

Catéter de dilatación para ACTP, Cathéter de dilatation pour ACTP, PTCA-Dilatationskatheter, Catetere dilatatore per PTCA, PTCA dilatatiekatheter, PTCA拡張カテーテル, PTCA-dilatationskateter, Καθετήρας διαστολής PTCA, Cateter de Dilatação para PTCA, PTCA-dilatationskateter, PTCA-tágítókatéter, Dilatační katétr pro PTCA, Cewnik rozszerzający do PTCA, PTCA-dilatasjonskateter, PTKA Dilatasyon Kateteri

| atm - kPa Pressure | | 2.0mm Balloon O.D. |
|---|---|---|
| 5.0 - 507 | | 1.97 |
| 6.0 - 608 | NOMINAL | 2.00 |
| 7.0 - 709 | | 2.03 |
| 8.0 - 811 | | 2.06 |
| 9.0 - 912 | | 2.09 |
| 10.0 - 1013 | | 2.12 |
| 11.0 - 1115 | | 2.15 |
| 12.0 - 1216 | RATED* | 2.19 |
| 13.0 - 1317 | | -- |
| 14.0 - 1419 | | -- |

*Rated Burst Pressure. DO NOT EXCEED.

Contents (1)




CL (1) Includes CLIPIT™ Hypotube Clip

GW R 0.014in (≤0.36mm) Recommended Guidewire

GC R 5F (≥0.058in/1.47mm) Recommended Guide Catheter

| | | | |
|---|---|---|---|
| **GTIN** | 08714729369967 | LOT | 12345678 |
| REF Catalog No. | H749389281220 0 | Use By | 2010-12-31 |

STERILE EO Sterilized using ethylene oxide.

90244533-01

Internal BSC Bar Code

92425134-10A

CE 0344

**Made in MALAYSIA**
PMT 741, Persiaran Cassia Selatan 1
Taman Perindustrian Batu Kawan
14110 Bandar Cassia,
Pulau Pinang, MALAYSIA

Boston Scientific
Maverick²™
2.0mm x 12mm
GTIN 08714729369967
REF H7493892812200
LOT 12345678

Boston Scientific
Maverick²™
2.0mm x 12mm
GTIN 08714729369967
REF H7493892812200
LOT 12345678

(01)08714729369967(17)101231(10)12345678 GS1

This product may be protected by one or more patents. Patent information can be obtained at http://www.bostonscientific.com/patents

**Label Specification Part Number:92425134-10A**

Boston Scientific

**2.25mm x 12mm**

# Maverick²™

## MONORAIL™


### PTCA Dilatation Catheter

Catéter de dilatación para ACTP, Cathéter de dilatation pour ACTP, PTCA-Dilatationskatheter, Catetere dilatatore per PTCA, PTCA dilatatiekatheter, PTCA拡張カテーテル, PTCA-dilatationskateter, Καθετήρας διαστολής PTCA, Cateter de Dilatação para PTCA, PTCA-dilatationskateter, PTCA-tágítókatéter, Dilatační katétr pro PTCA, Cewnik rozszerzający do PTCA, PTCA-dilatasjonskateter, PTKA Dilatasyon Kateteri

| atm - kPa Pressure | | 2.25mm Balloon O.D. |
|---|---|---|
| 5.0 - 507 | | 2.22 |
| 6.0 - 608 | NOMINAL | 2.25 |
| 7.0 - 709 | | 2.28 |
| 8.0 - 811 | | 2.31 |
| 9.0 - 912 | | 2.35 |
| 10.0 - 1013 | | 2.38 |
| 11.0 - 1115 | | 2.41 |
| 12.0 - 1216 | | 2.44 |
| 13.0 - 1317 | | 2.47 |
| 14.0 - 1419 | RATED* | 2.51 |

*Rated Burst Pressure and Stent Rated Burst Pressure. DO NOT EXCEED.

Contents (1)




CL (1) Includes CLIPIT™ Hypotube Clip

GW R 0.014in (≤0.36mm) Recommended Guidewire

GC R 5F (≥0.058in/1.47mm) Recommended Guide Catheter

| | | | |
|---|---|---|---|
| **GTIN** | 08714729369974 | LOT | 12345678 |
| REF Catalog No. | H7493892812220 | Use By | 2010-12-31 |

STERILE EO Sterilized using ethylene oxide.

90244533-01

Internal BSC Bar Code

92425134-11A

Boston Scientific
Maverick²™
2.25mm x 12mm
GTIN 08714729369974
REF H7493892812220
LOT 12345678

Boston Scientific
Maverick²™
2.25mm x 12mm
GTIN 08714729369974
REF H7493892812220
LOT 12345678

CE 0344

(01)08714729369974(17)101231(10)12345678 GS1

**Made in MALAYSIA**
PMT 741, Persiaran Cassia Selatan 1
Taman Perindustrian Batu Kawan
14110 Bandar Cassia,
Pulau Pinang, MALAYSIA

This product may be protected by one or more patents. Patent information can be obtained at http://www.bostonscientific.com/patents

**Label Specification Part Number:92425134-11A**

Boston Scientific

**2.5mm x 12mm**

# Maverick²™

## MONORAIL™


### PTCA Dilatation Catheter

Catéter de dilatación para ACTP, Cathéter de dilatation pour ACTP, PTCA-Dilatationskatheter, Catetere dilatatore per PTCA, PTCA dilatatiekatheter, PTCA拡張カテーテル, PTCA-dilatationskateter, Καθετήρας διαστολής PTCA, Cateter de Dilatação para PTCA, PTCA-dilatationskateter, PTCA-tágítókatéter, Dilatační katétr pro PTCA, Cewnik rozszerzający do PTCA, PTCA-dilatasjonskateter, PTKA Dilatasyon Kateteri

| atm - kPa Pressure | | 2.5mm Balloon O.D. |
|---|---|---|
| 5.0 - 507 | | 2.46 |
| 6.0 - 608 | NOMINAL | 2.50 |
| 7.0 - 709 | | 2.54 |
| 8.0 - 811 | | 2.58 |
| 9.0 - 912 | | 2.62 |
| 10.0 - 1013 | | 2.67 |
| 11.0 - 1115 | | 2.71 |
| 12.0 - 1216 | | 2.75 |
| 13.0 - 1317 | | 2.79 |
| 14.0 - 1419 | RATED* | 2.83 |

*Rated Burst Pressure and Stent Rated Burst Pressure. DO NOT EXCEED.

Contents (1)




CL (1) Includes CLIPIT™ Hypotube Clip

GW R 0.014in (≤0.36mm) Recommended Guidewire

GC R 5F (≥0.058in/1.47mm) Recommended Guide Catheter

| | | | |
|---|---|---|---|
| **GTIN** | 08714729369981 | LOT | 12345678 |
| REF Catalog No. | H749389281225 0 | Use By | 2010-12-31 |

STERILE EO Sterilized using ethylene oxide.

90244533-01

Internal BSC Bar Code

92425134-12A

CE 0344

**Made in MALAYSIA**
PMT 741, Persiaran Cassia Selatan 1
Taman Perindustrian Batu Kawan
14110 Bandar Cassia,
Pulau Pinang, MALAYSIA

Boston Scientific
Maverick²™
2.5mm x 12mm
GTIN 08714729369981
REF H7493892812250
LOT 12345678

Boston Scientific
Maverick²™
2.5mm x 12mm
GTIN 08714729369981
REF H7493892812250
LOT 12345678

(01)08714729369981(17)101231(10)12345678 GS1

This product may be protected by one or more patents. Patent information can be obtained at http://www.bostonscientific.com/patents

**Label Specification Part Number:92425134-12A**

Boston Scientific

2.75mm x12mm

# Maverick²™

## MONORAIL™


### PTCA Dilatation Catheter

Catéter de dilatación para ACTP, Cathéter de dilatation pour ACTP, PTCA-Dilatationskatheter, Catetere dilatatore per PTCA, PTCA dilatatiekatheter, PTCA拡張カテーテル, PTCA-dilatationskateter, Καθετήρας διαστολής PTCA, Cateter de Dilatação para PTCA, PTCA-dilatationskateter, PTCA-tágítókatéter, Dilatační katétr pro PTCA, Cewnik rozszerzający do PTCA, PTCA-dilatasjonskateter, PTKA Dilatasyon Kateteri

| atm - kPa Pressure | | 2.75mm Balloon O.D. |
|---|---|---|
| 5.0 - 507 | | 2.71 |
| 6.0 - 608 | NOMINAL | 2.75 |
| 7.0 - 709 | | 2.79 |
| 8.0 - 811 | | 2.83 |
| 9.0 - 912 | | 2.87 |
| 10.0 - 1013 | | 2.91 |
| 11.0 - 1115 | | 2.95 |
| 12.0 - 1216 | | 2.99 |
| 13.0 - 1317 | | 3.03 |
| 14.0 - 1419 | RATED* | 3.07 |

*Rated Burst Pressure and Stent Rated Burst Pressure. DO NOT EXCEED.

Contents (1)




CL (1) Includes CLIPIT™ Hypotube Clip

GW R 0.014in (≤0.36mm) Recommended Guidewire

GC R 5F (≥0.058in/1.47mm) Recommended Guide Catheter

| | | | |
|---|---|---|---|
| GTIN | 08714729369998 | LOT | 12345678 |
| REF Catalog No. | H749389281227o | Use By | 2010-12-31 |

STERILE EO Sterilized using ethylene oxide.

90244533-01

Internal BSC Bar Code

92425134-13A

CE 0344

**Made in MALAYSIA**
PMT 741, Persiaran Cassia Selatan 1
Taman Perindustrian Batu Kawan
14110 Bandar Cassia,
Pulau Pinang, MALAYSIA

Boston Scientific
Maverick²™
2.75mm x 12mm
GTIN 08714729369998
REF H7493892812270
LOT 12345678

Boston Scientific
Maverick²™
2.75mm x 12mm
GTIN 08714729369998
REF H7493892812270
LOT 12345678

(01)08714729369998(17)101231(10)12345678 GS1

This product may be protected by one or more patents. Patent information can be obtained at http://www.bostonscientific.com/patents

**Label Specification Part Number:92425134-13A**

Boston Scientific

**3.0mm x 12mm**

# Maverick²™

## MONORAIL™


### PTCA Dilatation Catheter

Catéter de dilatación para ACTP, Cathéter de dilatation pour ACTP, PTCA-Dilatationskatheter, Catetere dilatatore per PTCA, PTCA dilatatiekatheter, PTCA拡張カテーテル, PTCA-dilatationskateter, Καθετήρας διαστολής PTCA, Cateter de Dilatação para PTCA, PTCA-dilatationskateter, PTCA-tágítókatéter, Dilatační katétr pro PTCA, Cewnik rozszerzający do PTCA, PTCA-dilatasjonskateter, PTKA Dilatasyon Kateteri

| atm - kPa Pressure | | 3.0mm Balloon O.D. |
|---|---|---|
| 5.0 - 507 | | 2.95 |
| 6.0 - 608 | NOMINAL | 3.00 |
| 7.0 - 709 | | 3.05 |
| 8.0 - 811 | | 3.09 |
| 9.0 - 912 | | 3.14 |
| 10.0 - 1013 | | 3.18 |
| 11.0 - 1115 | | 3.23 |
| 12.0 - 1216 | | 3.28 |
| 13.0 - 1317 | | 3.32 |
| 14.0 - 1419 | RATED* | 3.37 |

*Rated Burst Pressure and Stent Rated Burst Pressure. DO NOT EXCEED.

Contents (1)




CL (1) Includes CLIPIT™ Hypotube Clip

GW R 0.014in (≤0.36mm) Recommended Guidewire

GC R 5F (≥0.058in/1.47mm) Recommended Guide Catheter

| | | | |
|---|---|---|---|
| **GTIN** | 08714729370000 | LOT | 12345678 |
| REF Catalog No. | H749389281230 0 | Use By | 2010-12-31 |

STERILE EO Sterilized using ethylene oxide.

90244533-01

Internal BSC Bar Code

92425134-14A

CE 0344

**Made in MALAYSIA**
PMT 741, Persiaran Cassia Selatan 1
Taman Perindustrian Batu Kawan
14110 Bandar Cassia,
Pulau Pinang, MALAYSIA

Boston Scientific
Maverick²™
3.0mm x 12mm
GTIN 08714729370000
REF H7493892812300
LOT 12345678

Boston Scientific
Maverick²™
3.0mm x 12mm
GTIN 08714729370000
REF H7493892812300
LOT 12345678

(01)08714729370000(17)101231(10)12345678 GS1

This product may be protected by one or more patents. Patent information can be obtained at http://www.bostonscientific.com/patents

**Label Specification Part Number:92425134-14A**

Boston Scientific

3.25mm x 12mm

# Maverick²™

## MONORAIL™


### PTCA Dilatation Catheter

Catéter de dilatación para ACTP, Cathéter de dilatation pour ACTP, PTCA-Dilatationskatheter, Catetere dilatatore per PTCA, PTCA dilatatiekatheter, PTCA拡張カテーテル, PTCA-dilatationskateter, Καθετήρας διαστολής PTCA, Cateter de Dilatação para PTCA, PTCA-dilatationskateter, PTCA-tágítókatéter, Dilatační katétr pro PTCA, Cewnik rozszerzający do PTCA, PTCA-dilatasjonskateter, PTKA Dilatasyon Kateteri

| atm - kPa Pressure | | 3.25mm Balloon O.D. |
|---|---|---|
| 5.0 - 507 | | 3.20 |
| 6.0 - 608 | NOMINAL | 3.25 |
| 7.0 - 709 | | 3.30 |
| 8.0 - 811 | | 3.34 |
| 9.0 - 912 | | 3.39 |
| 10.0 - 1013 | | 3.43 |
| 11.0 - 1115 | | 3.48 |
| 12.0 - 1216 | | 3.52 |
| 13.0 - 1317 | | 3.57 |
| 14.0 - 1419 | RATED* | 3.61 |

*Rated Burst Pressure and Stent Rated Burst Pressure. DO NOT EXCEED.

Contents (1)




CL (1) Includes CLIPIT™ Hypotube Clip

GW R 0.014in (≤0.36mm) Recommended Guidewire

GC R 5F (≥0.058in/1.47mm) Recommended Guide Catheter

| | | | |
|---|---|---|---|
| GTIN | 08714729370017 | LOT | 12345678 |
| REF Catalog No. | H749389281232 0 | Use By | 2010-12-31 |

STERILE EO Sterilized using ethylene oxide.

90244533-01

Internal BSC Bar Code

92425134-15A

CE 0344

**Made in MALAYSIA**
PMT 741, Persiaran Cassia Selatan 1
Taman Perindustrian Batu Kawan
14110 Bandar Cassia,
Pulau Pinang, MALAYSIA

Boston Scientific
Maverick²™
3.25mm x 12mm
GTIN 08714729370017
REF H7493892812320
LOT 12345678

Boston Scientific
Maverick²™
3.25mm x 12mm
GTIN 08714729370017
REF H7493892812320
LOT 12345678

(01)08714729370017(17)101231(10)12345678 GS1

This product may be protected by one or more patents. Patent information can be obtained at http://www.bostonscientific.com/patents

**Label Specification Part Number:92425134-15A**

Boston Scientific

3.5mm x 12mm

# Maverick²™

## MONORAIL™


### PTCA Dilatation Catheter

Catéter de dilatación para ACTP, Cathéter de dilatation pour ACTP, PTCA-Dilatationskatheter, Catetere dilatatore per PTCA, PTCA dilatatiekatheter, PTCA拡張カテーテル, PTCA-dilatationskateter, Καθετήρας διαστολής PTCA, Cateter de Dilatação para PTCA, PTCA-dilatationskateter, PTCA-tágítókatéter, Dilatační katétr pro PTCA, Cewnik rozszerzający do PTCA, PTCA-dilatasjonskateter, PTKA Dilatasyon Kateteri

| atm - kPa Pressure | | 3.5mm Balloon O.D. |
|---|---|---|
| 5.0 - 507 | | 3.45 |
| 6.0 - 608 | NOMINAL | 3.50 |
| 7.0 - 709 | | 3.55 |
| 8.0 - 811 | | 3.60 |
| 9.0 - 912 | | 3.65 |
| 10.0 - 1013 | | 3.71 |
| 11.0 - 1115 | | 3.76 |
| 12.0 - 1216 | RATED* | 3.81 |
| 13.0 - 1317 | | -- |
| 14.0 - 1419 | | -- |

*Rated Burst Pressure and Stent Rated Burst Pressure. DO NOT EXCEED.

Contents (1)




CL (1) Includes CLIPIT™ Hypotube Clip

GW R 0.014in (≤0.36mm) Recommended Guidewire

GC R 5F (≥0.058in/1.47mm) Recommended Guide Catheter

| | | | |
|---|---|---|---|
| **GTIN** | 08714729370024 | LOT | 12345678 |
| REF Catalog No. | H7493892812350 | Use By | 2010-12-31 |

STERILE EO Sterilized using ethylene oxide.

90244533-01

Internal BSC Bar Code

92425134-16A

CE 0344

**Made in MALAYSIA**
PMT 741, Persiaran Cassia Selatan 1
Taman Perindustrian Batu Kawan
14110 Bandar Cassia,
Pulau Pinang, MALAYSIA

Boston Scientific
Maverick²™
3.5mm x 12mm
GTIN 08714729370024
REF H7493892812350
LOT 12345678

Boston Scientific
Maverick²™
3.5mm x 12mm
GTIN 08714729370024
REF H7493892812350
LOT 12345678

(01)08714729370024(17)101231(10)12345678 GS1

This product may be protected by one or more patents. Patent information can be obtained at http://www.bostonscientific.com/patents

**Label Specification Part Number:92425134-16A**

Boston Scientific

**3.75mm x 12mm**

# Maverick²™

## MONORAIL™


### PTCA Dilatation Catheter

Catéter de dilatación para ACTP, Cathéter de dilatation pour ACTP, PTCA-Dilatationskatheter, Catetere dilatatore per PTCA, PTCA dilatatiekatheter, PTCA拡張カテーテル, PTCA-dilatationskateter, Καθετήρας διαστολής PTCA, Cateter de Dilatação para PTCA, PTCA-dilatationskateter, PTCA-tágítókatéter, Dilatační katétr pro PTCA, Cewnik rozszerzający do PTCA, PTCA-dilatasjonskateter, PTKA Dilatasyon Kateteri

| atm - kPa Pressure | | 3.75mm Balloon O.D. |
|---|---|---|
| 5.0 - 507 | | 3.70 |
| 6.0 - 608 | NOMINAL | 3.75 |
| 7.0 - 709 | | 3.80 |
| 8.0 - 811 | | 3.85 |
| 9.0 - 912 | | 3.90 |
| 10.0 - 1013 | | 3.95 |
| 11.0 - 1115 | | 4.00 |
| 12.0 - 1216 | RATED* | 4.05 |
| 13.0 - 1317 | | -- |
| 14.0 - 1419 | | -- |

*Rated Burst Pressure and Stent Rated Burst Pressure. DO NOT EXCEED.

Contents (1)




CL (1) Includes CLIPIT™ Hypotube Clip

GW R 0.014in (≤0.36mm) Recommended Guidewire

GC R 5F (≥0.058in/1.47mm) Recommended Guide Catheter

| | | | |
|---|---|---|---|
| **GTIN** | 08714729370031 | LOT | 12345678 |
| REF Catalog No. | H749389281237o | Use By | 2010-12-31 |

STERILE EO Sterilized using ethylene oxide.

90244533-01

Internal BSC Bar Code

92425134-17A

CE 0344

**Made in MALAYSIA**
PMT 741, Persiaran Cassia Selatan 1
Taman Perindustrian Batu Kawan
14110 Bandar Cassia,
Pulau Pinang, MALAYSIA

Boston Scientific
Maverick²™
3.75mm x 12mm
GTIN 08714729370031
REF H7493892812370
LOT 12345678

Boston Scientific
Maverick²™
3.75mm x 12mm
GTIN 08714729370031
REF H7493892812370
LOT 12345678

(01)08714729370031(17)101231(10)12345678 GS1

This product may be protected by one or more patents. Patent information can be obtained at http://www.bostonscientific.com/patents

**Label Specification Part Number:92425134-17A**

Boston Scientific

**4.0mm x 12mm**

# Maverick²™

## MONORAIL™


### PTCA Dilatation Catheter

Catéter de dilatación para ACTP, Cathéter de dilatation pour ACTP, PTCA-Dilatationskatheter, Catetere dilatatore per PTCA, PTCA dilatatiekatheter, PTCA拡張カテーテル, PTCA-dilatationskateter, Καθετήρας διαστολής PTCA, Cateter de Dilatação para PTCA, PTCA-dilatationskateter, PTCA-tágítókatéter, Dilatační katétr pro PTCA, Cewnik rozszerzający do PTCA, PTCA-dilatasjonskateter, PTKA Dilatasyon Kateteri

| atm - kPa Pressure | | 4.0mm Balloon O.D. |
|---|---|---|
| 5.0 - 507 | | 3.95 |
| 6.0 - 608 | NOMINAL | 4.00 |
| 7.0 - 709 | | 4.05 |
| 8.0 - 811 | | 4.10 |
| 9.0 - 912 | | 4.15 |
| 10.0 - 1013 | | 4.20 |
| 11.0 - 1115 | | 4.25 |
| 12.0 - 1216 | RATED* | 4.31 |
| 13.0 - 1317 | | -- |
| 14.0 - 1419 | | -- |

*Rated Burst Pressure and Stent Rated Burst Pressure. DO NOT EXCEED.

Contents (1)




CL (1) Includes CLIPIT™ Hypotube Clip

GW R 0.014in (≤0.36mm) Recommended Guidewire

GC R 5F (≥0.058in/1.47mm) Recommended Guide Catheter

| | | | |
|---|---|---|---|
| **GTIN** | 08714729370048 | LOT | 12345678 |
| REF Catalog No. | H749389281240 0 | Use By | 2010-12-31 |

STERILE EO Sterilized using ethylene oxide.

90244533-01

Internal BSC Bar Code

92425134-18A

CE 0344

**Made in MALAYSIA**
PMT 741, Persiaran Cassia Selatan 1
Taman Perindustrian Batu Kawan
14110 Bandar Cassia,
Pulau Pinang, MALAYSIA

Boston Scientific
Maverick²™
4.0mm x 12mm
GTIN 08714729370048
REF H7493892812400
LOT 12345678

Boston Scientific
Maverick²™
4.0mm x 12mm
GTIN 08714729370048
REF H7493892812400
LOT 12345678

(01)08714729370048(17)101231(10)12345678 GS1

This product may be protected by one or more patents. Patent information can be obtained at http://www.bostonscientific.com/patents

**Label Specification Part Number:92425134-18A**

Boston Scientific

1.5mm x 15mm

# Maverick²™

## MONORAIL™


### PTCA Dilatation Catheter

Catéter de dilatación para ACTP, Cathéter de dilatation pour ACTP, PTCA-Dilatationskatheter, Catetere dilatatore per PTCA, PTCA dilatatiekatheter, PTCA拡張カテーテル, PTCA-dilatationskateter, Καθετήρας διαστολής PTCA, Cateter de Dilatação para PTCA, PTCA-dilatationskateter, PTCA-tágítókatéter, Dilatační katétr pro PTCA, Cewnik rozszerzający do PTCA, PTCA-dilatasjonskateter, PTKA Dilatasyon Kateteri

| atm - kPa Pressure | | 1.5mm Balloon O.D. |
|---|---|---|
| 5.0 - 507 | | 1.48 |
| 6.0 - 608 | NOMINAL | 1.50 |
| 7.0 - 709 | | 1.52 |
| 8.0 - 811 | | 1.55 |
| 9.0 - 912 | | 1.57 |
| 10.0 - 1013 | | 1.59 |
| 11.0 - 1115 | | 1.61 |
| 12.0 - 1216 | RATED* | 1.63 |
| 13.0 - 1317 | | -- |
| 14.0 - 1419 | | -- |

*Rated Burst Pressure. DO NOT EXCEED.

Contents (1)

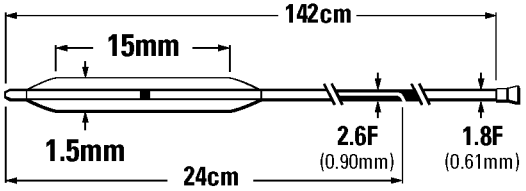


CL (1) Includes CLIPIT™ Hypotube Clip

GW R 0.014in (≤0.36mm) Recommended Guidewire

GC R 5F (≥0.058in/1.47mm) Recommended Guide Catheter

| | | | |
|---|---|---|---|
| GTIN | 08714729370055 | LOT | 12345678 |
| REF Catalog No. | H7493892815150 | Use By | 2010-12-31 |

STERILE EO Sterilized using ethylene oxide.

90244533-01

Internal BSC Bar Code

92425134-19A

CE 0344

**Made in MALAYSIA**
PMT 741, Persiaran Cassia Selatan 1
Taman Perindustrian Batu Kawan
14110 Bandar Cassia,
Pulau Pinang, MALAYSIA

Boston Scientific
Maverick²™
1.5mm x 15mm
GTIN 08714729370055
REF H7493892815150
LOT 12345678

Boston Scientific
Maverick²™
1.5mm x 15mm
GTIN 08714729370055
REF H7493892815150
LOT 12345678

(01)08714729370055(17)101231(10)12345678 GS1

This product may be protected by one or more patents. Patent information can be obtained at http://www.bostonscientific.com/patents

**Label Specification Part Number:92425134-19A**

Boston Scientific

**2.0mm x 15mm**

# Maverick²™

## MONORAIL™


### PTCA Dilatation Catheter

Catéter de dilatación para ACTP, Cathéter de dilatation pour ACTP, PTCA-Dilatationskatheter, Catetere dilatatore per PTCA, PTCA dilatatiekatheter, PTCA拡張カテーテル, PTCA-dilatationskateter, Καθετήρας διαστολής PTCA, Cateter de Dilatação para PTCA, PTCA-dilatationskateter, PTCA-tágítókatéter, Dilatační katétr pro PTCA, Cewnik rozszerzający do PTCA, PTCA-dilatasjonskateter, PTKA Dilatasyon Kateteri

| atm - kPa Pressure | | 2.0mm Balloon O.D. |
|---|---|---|
| 5.0 - 507 | | 1.97 |
| 6.0 - 608 | NOMINAL | 2.00 |
| 7.0 - 709 | | 2.03 |
| 8.0 - 811 | | 2.06 |
| 9.0 - 912 | | 2.09 |
| 10.0 - 1013 | | 2.12 |
| 11.0 - 1115 | | 2.15 |
| 12.0 - 1216 | RATED* | 2.19 |
| 13.0 - 1317 | | -- |
| 14.0 - 1419 | | -- |

*Rated Burst Pressure. DO NOT EXCEED.

Contents (1)




CL (1) Includes CLIPIT™ Hypotube Clip

GW R 0.014in (≤0.36mm) Recommended Guidewire

GC R 5F (≥0.058in/1.47mm) Recommended Guide Catheter

| | | | |
|---|---|---|---|
| **GTIN** | 08714729370062 | LOT | 12345678 |
| REF Catalog No. | H749389281520 0 | Use By | 2010-12-31 |

STERILE EO Sterilized using ethylene oxide.

90244533-01

Internal BSC Bar Code

92425134-20A

CE 0344

**Made in MALAYSIA**
PMT 741, Persiaran Cassia Selatan 1
Taman Perindustrian Batu Kawan
14110 Bandar Cassia,
Pulau Pinang, MALAYSIA

Boston Scientific
Maverick²™
2.0mm x 15mm
GTIN 08714729370062
REF H7493892815200
LOT 12345678

Boston Scientific
Maverick²™
2.0mm x 15mm
GTIN 08714729370062
REF H7493892815200
LOT 12345678

(01)08714729370062(17)101231(10)12345678 GS1

This product may be protected by one or more patents. Patent information can be obtained at http://www.bostonscientific.com/patents

**Label Specification Part Number:92425134-20A**

Boston Scientific

2.25mm x 15mm

# Maverick²™

## MONORAIL™


### PTCA Dilatation Catheter

Catéter de dilatación para ACTP, Cathéter de dilatation pour ACTP, PTCA-Dilatationskatheter, Catetere dilatatore per PTCA, PTCA dilatatiekatheter, PTCA拡張カテーテル, PTCA-dilatationskateter, Καθετήρας διαστολής PTCA, Cateter de Dilatação para PTCA, PTCA-dilatationskateter, PTCA-tágítókatéter, Dilatační katétr pro PTCA, Cewnik rozszerzający do PTCA, PTCA-dilatasjonskateter, PTKA Dilatasyon Kateteri

| atm - kPa Pressure | | 2.25mm Balloon O.D. |
|---|---|---|
| 5.0 - 507 | | 2.22 |
| 6.0 - 608 | NOMINAL | 2.25 |
| 7.0 - 709 | | 2.28 |
| 8.0 - 811 | | 2.31 |
| 9.0 - 912 | | 2.35 |
| 10.0 - 1013 | | 2.38 |
| 11.0 - 1115 | | 2.41 |
| 12.0 - 1216 | | 2.44 |
| 13.0 - 1317 | | 2.47 |
| 14.0 - 1419 | RATED* | 2.51 |

*Rated Burst Pressure and Stent Rated Burst Pressure. DO NOT EXCEED.

Contents (1)




CL (1) Includes CLIPIT™ Hypotube Clip

GW R 0.014in (≤0.36mm) Recommended Guidewire

GC R 5F (≥0.058in/1.47mm) Recommended Guide Catheter

| | | | |
|---|---|---|---|
| GTIN | 08714729370079 | LOT | 12345678 |
| REF Catalog No. | H7493892815220 | Use By | 2010-12-31 |

STERILE EO Sterilized using ethylene oxide.

90244533-01

Internal BSC Bar Code

92425134-21A

CE 0344

Made in MALAYSIA
PMT 741, Persiaran Cassia Selatan 1
Taman Perindustrian Batu Kawan
14110 Bandar Cassia,
Pulau Pinang, MALAYSIA

Boston Scientific
Maverick²™
2.25mm x 15mm
GTIN 08714729370079
REF H7493892815220
LOT 12345678

Boston Scientific
Maverick²™
2.25mm x 15mm
GTIN 08714729370079
REF H7493892815220
LOT 12345678

(01)08714729370079(17)101231(10)12345678 GS1

This product may be protected by one or more patents. Patent information can be obtained at http://www.bostonscientific.com/patents

**Label Specification Part Number:92425134-21A**

Boston Scientific

**2.5mm x 15mm**

# Maverick²™

## MONORAIL™


### PTCA Dilatation Catheter

Catéter de dilatación para ACTP, Cathéter de dilatation pour ACTP, PTCA-Dilatationskatheter, Catetere dilatatore per PTCA, PTCA dilatatiekatheter, PTCA拡張カテーテル, PTCA-dilatationskateter, Καθετήρας διαστολής PTCA, Cateter de Dilatação para PTCA, PTCA-dilatationskateter, PTCA-tágítókatéter, Dilatační katétr pro PTCA, Cewnik rozszerzający do PTCA, PTCA-dilatasjonskateter, PTKA Dilatasyon Kateteri

| atm - kPa Pressure | | 2.5mm Balloon O.D. |
|---|---|---|
| 5.0 - 507 | | 2.46 |
| 6.0 - 608 | NOMINAL | 2.50 |
| 7.0 - 709 | | 2.54 |
| 8.0 - 811 | | 2.58 |
| 9.0 - 912 | | 2.62 |
| 10.0 - 1013 | | 2.67 |
| 11.0 - 1115 | | 2.71 |
| 12.0 - 1216 | | 2.75 |
| 13.0 - 1317 | | 2.79 |
| 14.0 - 1419 | RATED* | 2.83 |

*Rated Burst Pressure and Stent Rated Burst Pressure. DO NOT EXCEED.

Contents (1)




CL (1) Includes CLIPIT™ Hypotube Clip

GW R 0.014in (≤0.36mm) Recommended Guidewire

GC R 5F (≥0.058in/1.47mm) Recommended Guide Catheter

| | | | |
|---|---|---|---|
| **GTIN** | 08714729370086 | LOT | 12345678 |
| REF Catalog No. | H7493892815250 | Use By | 2010-12-31 |

STERILE EO Sterilized using ethylene oxide.

90244533-01

Internal BSC Bar Code

92425134-22A

CE 0344

**Made in MALAYSIA**
PMT 741, Persiaran Cassia Selatan 1
Taman Perindustrian Batu Kawan
14110 Bandar Cassia,
Pulau Pinang, MALAYSIA

Boston Scientific
Maverick²™
2.5mm x 15mm
GTIN 08714729370086
REF H7493892815250
LOT 12345678

Boston Scientific
Maverick²™
2.5mm x 15mm
GTIN 08714729370086
REF H7493892815250
LOT 12345678

(01)08714729370086(17)101231(10)12345678 GS1

This product may be protected by one or more patents. Patent information can be obtained at http://www.bostonscientific.com/patents

**Label Specification Part Number:92425134-22A**

Boston Scientific

**2.75mm x 15mm**

# Maverick²™

## MONORAIL™


### PTCA Dilatation Catheter

Catéter de dilatación para ACTP, Cathéter de dilatation pour ACTP, PTCA-Dilatationskatheter, Catetere dilatatore per PTCA, PTCA dilatatiekatheter, PTCA拡張カテーテル, PTCA-dilatationskateter, Καθετήρας διαστολής PTCA, Cateter de Dilatação para PTCA, PTCA-dilatationskateter, PTCA-tágítókatéter, Dilatační katétr pro PTCA, Cewnik rozszerzający do PTCA, PTCA-dilatasjonskateter, PTKA Dilatasyon Kateteri

| atm - kPa Pressure | | 2.75mm Balloon O.D. |
|---|---|---|
| 5.0 - 507 | | 2.71 |
| 6.0 - 608 | NOMINAL | 2.75 |
| 7.0 - 709 | | 2.79 |
| 8.0 - 811 | | 2.83 |
| 9.0 - 912 | | 2.87 |
| 10.0 - 1013 | | 2.91 |
| 11.0 - 1115 | | 2.95 |
| 12.0 - 1216 | | 2.99 |
| 13.0 - 1317 | | 3.03 |
| 14.0 - 1419 | RATED* | 3.07 |

*Rated Burst Pressure and Stent Rated Burst Pressure. DO NOT EXCEED.

Contents (1)




CL (1) Includes CLIPIT™ Hypotube Clip

GW R 0.014in (≤0.36mm) Recommended Guidewire

GC R 5F (≥0.058in/1.47mm) Recommended Guide Catheter

| | | | |
|---|---|---|---|
| **GTIN** | 08714729370093 | LOT | 12345678 |
| REF Catalog No. | H7493892815270 | Use By | 2010-12-31 |

STERILE EO Sterilized using ethylene oxide.

90244533-01

Internal BSC Bar Code

92425134-23A

Boston Scientific
Maverick²™
2.75mm x 15mm
GTIN 08714729370093
REF H7493892815270
LOT 12345678

Boston Scientific
Maverick²™
2.75mm x 15mm
GTIN 08714729370093
REF H7493892815270
LOT 12345678

CE 0344

(01)08714729370093(17)101231(10)12345678 GS1

**Made in MALAYSIA**
PMT 741, Persiaran Cassia Selatan 1
Taman Perindustrian Batu Kawan
14110 Bandar Cassia,
Pulau Pinang, MALAYSIA

This product may be protected by one or more patents. Patent information can be obtained at http://www.bostonscientific.com/patents

**Label Specification Part Number:92425134-23A**

Boston Scientific

**3.0mm x 15mm**

# Maverick²™

## MONORAIL™


### PTCA Dilatation Catheter

Catéter de dilatación para ACTP, Cathéter de dilatation pour ACTP, PTCA-Dilatationskatheter, Catetere dilatatore per PTCA, PTCA dilatatiekatheter, PTCA拡張カテーテル, PTCA-dilatationskateter, Καθετήρας διαστολής PTCA, Cateter de Dilatação para PTCA, PTCA-dilatationskateter, PTCA-tágítókatéter, Dilatační katétr pro PTCA, Cewnik rozszerzający do PTCA, PTCA-dilatasjonskateter, PTKA Dilatasyon Kateteri

| atm - kPa Pressure | | 3.0mm Balloon O.D. |
|---|---|---|
| 5.0 - 507 | | 2.95 |
| 6.0 - 608 | NOMINAL | 3.00 |
| 7.0 - 709 | | 3.05 |
| 8.0 - 811 | | 3.09 |
| 9.0 - 912 | | 3.14 |
| 10.0 - 1013 | | 3.18 |
| 11.0 - 1115 | | 3.23 |
| 12.0 - 1216 | | 3.28 |
| 13.0 - 1317 | | 3.32 |
| 14.0 - 1419 | RATED* | 3.37 |

*Rated Burst Pressure and Stent Rated Burst Pressure. DO NOT EXCEED.

Contents (1)




CL (1) Includes CLIPIT™ Hypotube Clip

GW R 0.014in (≤0.36mm) Recommended Guidewire

GC R 5F (≥0.058in/1.47mm) Recommended Guide Catheter

| | | | |
|---|---|---|---|
| **GTIN** | 08714729370109 | LOT | 12345678 |
| REF Catalog No. | H7493892815300 | Use By | 2010-12-31 |

STERILE EO Sterilized using ethylene oxide.

90244533-01

Internal BSC Bar Code

92425134-24A

CE 0344

**Made in MALAYSIA**
PMT 741, Persiaran Cassia Selatan 1
Taman Perindustrian Batu Kawan
14110 Bandar Cassia,
Pulau Pinang, MALAYSIA

Boston Scientific
Maverick²™
3.0mm x 15mm
GTIN 08714729370109
REF H7493892815300
LOT 12345678

Boston Scientific
Maverick²™
3.0mm x 15mm
GTIN 08714729370109
REF H7493892815300
LOT 12345678

(01)08714729370109(17)101231(10)12345678 GS1

This product may be protected by one or more patents. Patent information can be obtained at http://www.bostonscientific.com/patents

**Label Specification Part Number:92425134-24A**

Boston Scientific

3.25mm x 15mm

# Maverick²™

## MONORAIL™


### PTCA Dilatation Catheter

Catéter de dilatación para ACTP, Cathéter de dilatation pour ACTP, PTCA-Dilatationskatheter, Catetere dilatatore per PTCA, PTCA dilatatiekatheter, PTCA拡張カテーテル, PTCA-dilatationskateter, Καθετήρας διαστολής PTCA, Cateter de Dilatação para PTCA, PTCA-dilatationskateter, PTCA-tágítókatéter, Dilatační katétr pro PTCA, Cewnik rozszerzający do PTCA, PTCA-dilatasjonskateter, PTKA Dilatasyon Kateteri

| atm - kPa Pressure | | 3.25mm Balloon O.D. |
|---|---|---|
| 5.0 - 507 | | 3.20 |
| 6.0 - 608 | NOMINAL | 3.25 |
| 7.0 - 709 | | 3.30 |
| 8.0 - 811 | | 3.34 |
| 9.0 - 912 | | 3.39 |
| 10.0 - 1013 | | 3.43 |
| 11.0 - 1115 | | 3.48 |
| 12.0 - 1216 | | 3.52 |
| 13.0 - 1317 | | 3.57 |
| 14.0 - 1419 | RATED* | 3.61 |

*Rated Burst Pressure and Stent Rated Burst Pressure. DO NOT EXCEED.

Contents (1)




CL (1) Includes CLIPIT™ Hypotube Clip

GW R 0.014in (≤0.36mm) Recommended Guidewire

GC R 5F (≥0.058in/1.47mm) Recommended Guide Catheter

| | | | |
|---|---|---|---|
| **GTIN** | 08714729370116 | LOT | 12345678 |
| REF Catalog No. | H749389281532 0 | Use By | 2010-12-31 |

STERILE EO Sterilized using ethylene oxide.

90244533-01

Internal BSC Bar Code

92425134-25A

CE 0344

**Made in MALAYSIA**
PMT 741, Persiaran Cassia Selatan 1
Taman Perindustrian Batu Kawan
14110 Bandar Cassia,
Pulau Pinang, MALAYSIA

Boston Scientific
Maverick²™
3.25mm x 15mm
GTIN 08714729370116
REF H7493892815320
LOT 12345678

Boston Scientific
Maverick²™
3.25mm x 15mm
GTIN 08714729370116
REF H7493892815320
LOT 12345678

(01)08714729370116(17)101231(10)12345678 GS1

This product may be protected by one or more patents. Patent information can be obtained at http://www.bostonscientific.com/patents

**Label Specification Part Number:92425134-25A**

Boston Scientific

**3.5mm x 15mm**

# Maverick²™

## MONORAIL™


### PTCA Dilatation Catheter

Catéter de dilatación para ACTP, Cathéter de dilatation pour ACTP, PTCA-Dilatationskatheter, Catetere dilatatore per PTCA, PTCA dilatatiekatheter, PTCA拡張カテーテル, PTCA-dilatationskateter, Καθετήρας διαστολής PTCA, Cateter de Dilatação para PTCA, PTCA-dilatationskateter, PTCA-tágítókatéter, Dilatační katétr pro PTCA, Cewnik rozszerzający do PTCA, PTCA-dilatasjonskateter, PTKA Dilatasyon Kateteri

| atm - kPa Pressure | | 3.5mm Balloon O.D. |
|---|---|---|
| 5.0 - 507 | | 3.45 |
| 6.0 - 608 | NOMINAL | 3.50 |
| 7.0 - 709 | | 3.55 |
| 8.0 - 811 | | 3.60 |
| 9.0 - 912 | | 3.65 |
| 10.0 - 1013 | | 3.71 |
| 11.0 - 1115 | | 3.76 |
| 12.0 - 1216 | RATED* | 3.81 |
| 13.0 - 1317 | | -- |
| 14.0 - 1419 | | -- |

*Rated Burst Pressure and Stent Rated Burst Pressure. DO NOT EXCEED.

Contents (1)




CL (1) Includes CLIPIT™ Hypotube Clip

GW R 0.014in (≤0.36mm) Recommended Guidewire

GC R 5F (≥0.058in/1.47mm) Recommended Guide Catheter

| | | | |
|---|---|---|---|
| **GTIN** | 08714729370123 | LOT | 12345678 |
| REF Catalog No. | H7493892815350 | Use By | 2010-12-31 |

STERILE EO Sterilized using ethylene oxide.

90244533-01

Internal BSC Bar Code

92425134-26A

Boston Scientific
Maverick²™
3.5mm x 15mm
GTIN 08714729370123
REF H7493892815350
LOT 12345678

Boston Scientific
Maverick²™
3.5mm x 15mm
GTIN 08714729370123
REF H7493892815350
LOT 12345678

CE 0344

(01)08714729370123(17)101231(10)12345678 GS1

**Made in MALAYSIA**
PMT 741, Persiaran Cassia Selatan 1
Taman Perindustrian Batu Kawan
14110 Bandar Cassia,
Pulau Pinang, MALAYSIA

This product may be protected by one or more patents. Patent information can be obtained at http://www.bostonscientific.com/patents

**Label Specification Part Number:92425134-26A**

Boston Scientific

**3.75mm x 15mm**

# Maverick²™

## MONORAIL™


### PTCA Dilatation Catheter

Catéter de dilatación para ACTP, Cathéter de dilatation pour ACTP, PTCA-Dilatationskatheter, Catetere dilatatore per PTCA, PTCA dilatatiekatheter, PTCA拡張カテーテル, PTCA-dilatationskateter, Καθετήρας διαστολής PTCA, Cateter de Dilatação para PTCA, PTCA-dilatationskateter, PTCA-tágítókatéter, Dilatační katétr pro PTCA, Cewnik rozszerzający do PTCA, PTCA-dilatasjonskateter, PTKA Dilatasyon Kateteri

| atm - kPa Pressure | | 3.75mm Balloon O.D. |
|---|---|---|
| 5.0 - 507 | | 3.70 |
| 6.0 - 608 | NOMINAL | 3.75 |
| 7.0 - 709 | | 3.80 |
| 8.0 - 811 | | 3.85 |
| 9.0 - 912 | | 3.90 |
| 10.0 - 1013 | | 3.95 |
| 11.0 - 1115 | | 4.00 |
| 12.0 - 1216 | RATED* | 4.05 |
| 13.0 - 1317 | | -- |
| 14.0 - 1419 | | -- |

*Rated Burst Pressure and Stent Rated Burst Pressure. DO NOT EXCEED.

Contents (1)




CL (1) Includes CLIPIT™ Hypotube Clip

GW R 0.014in (≤0.36mm) Recommended Guidewire

GC R 5F (≥0.058in/1.47mm) Recommended Guide Catheter

| | | | |
|---|---|---|---|
| **GTIN** | 08714729370130 | LOT | 12345678 |
| REF Catalog No. | H749389281537o | Use By | 2010-12-31 |

STERILE EO Sterilized using ethylene oxide.

90244533-01

Internal BSC Bar Code

92425134-27A

CE 0344

**Made in MALAYSIA**
PMT 741, Persiaran Cassia Selatan 1
Taman Perindustrian Batu Kawan
14110 Bandar Cassia,
Pulau Pinang, MALAYSIA

Boston Scientific
Maverick²™
3.75mm x 15mm
GTIN 08714729370130
REF H7493892815370
LOT 12345678

Boston Scientific
Maverick²™
3.75mm x 15mm
GTIN 08714729370130
REF H7493892815370
LOT 12345678

(01)08714729370130(17)101231(10)12345678 GS1

This product may be protected by one or more patents. Patent information can be obtained at http://www.bostonscientific.com/patents

**Label Specification Part Number:92425134-27A**

Boston Scientific

**4.0mm x 15mm**

# Maverick²™

## MONORAIL™


### PTCA Dilatation Catheter

Catéter de dilatación para ACTP, Cathéter de dilatation pour ACTP, PTCA-Dilatationskatheter, Catetere dilatatore per PTCA, PTCA dilatatiekatheter, PTCA拡張カテーテル, PTCA-dilatationskateter, Καθετήρας διαστολής PTCA, Cateter de Dilatação para PTCA, PTCA-dilatationskateter, PTCA-tágítókatéter, Dilatační katétr pro PTCA, Cewnik rozszerzający do PTCA, PTCA-dilatasjonskateter, PTKA Dilatasyon Kateteri

| atm - kPa Pressure | | 4.0mm Balloon O.D. |
|---|---|---|
| 5.0 - 507 | | 3.95 |
| 6.0 - 608 | NOMINAL | 4.00 |
| 7.0 - 709 | | 4.05 |
| 8.0 - 811 | | 4.10 |
| 9.0 - 912 | | 4.15 |
| 10.0 - 1013 | | 4.20 |
| 11.0 - 1115 | | 4.25 |
| 12.0 - 1216 | RATED* | 4.31 |
| 13.0 - 1317 | | -- |
| 14.0 - 1419 | | -- |

*Rated Burst Pressure and Stent Rated Burst Pressure. DO NOT EXCEED.

Contents (1)




CL (1) Includes CLIPIT™ Hypotube Clip

GW R 0.014in (≤0.36mm) Recommended Guidewire

GC R 5F (≥0.058in/1.47mm) Recommended Guide Catheter

| | | | |
|---|---|---|---|
| **GTIN** | 08714729370147 | LOT | 12345678 |
| REF Catalog No. | H749389281540o | Use By | 2010-12-31 |

STERILE EO Sterilized using ethylene oxide.

90244533-01

Internal BSC Bar Code

92425134-28A

CE 0344

**Made in MALAYSIA**
PMT 741, Persiaran Cassia Selatan 1
Taman Perindustrian Batu Kawan
14110 Bandar Cassia,
Pulau Pinang, MALAYSIA

Boston Scientific
Maverick²™
4.0mm x 15mm
GTIN 08714729370147
REF H7493892815400
LOT 12345678

Boston Scientific
Maverick²™
4.0mm x 15mm
GTIN 08714729370147
REF H7493892815400
LOT 12345678

(01)08714729370147(17)101231(10)12345678 GS1

This product may be protected by one or more patents. Patent information can be obtained at http://www.bostonscientific.com/patents

**Label Specification Part Number:92425134-28A**

Boston Scientific

1.5mm x 20mm

# Maverick²™

## MONORAIL™


### PTCA Dilatation Catheter

Catéter de dilatación para ACTP, Cathéter de dilatation pour ACTP, PTCA-Dilatationskatheter, Catetere dilatatore per PTCA, PTCA dilatatiekatheter, PTCA拡張カテーテル, PTCA-dilatationskateter, Καθετήρας διαστολής PTCA, Cateter de Dilatação para PTCA, PTCA-dilatationskateter, PTCA-tágítókatéter, Dilatační katétr pro PTCA, Cewnik rozszerzający do PTCA, PTCA-dilatasjonskateter, PTKA Dilatasyon Kateteri

| atm - kPa Pressure | | 1.5mm Balloon O.D. |
|---|---|---|
| 5.0 - 507 | | 1.48 |
| 6.0 - 608 | NOMINAL | 1.50 |
| 7.0 - 709 | | 1.52 |
| 8.0 - 811 | | 1.55 |
| 9.0 - 912 | | 1.57 |
| 10.0 - 1013 | | 1.59 |
| 11.0 - 1115 | | 1.61 |
| 12.0 - 1216 | RATED* | 1.63 |
| 13.0 - 1317 | | -- |
| 14.0 - 1419 | | -- |

*Rated Burst Pressure. DO NOT EXCEED.

Contents (1)

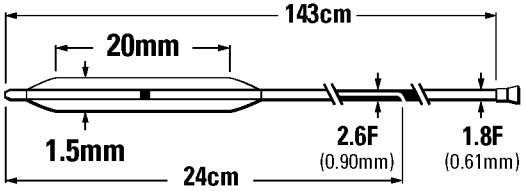


CL (1) Includes CLIPIT™ Hypotube Clip

GW R 0.014in (≤0.36mm) Recommended Guidewire

GC R 5F (≥0.058in/1.47mm) Recommended Guide Catheter

| | | | |
|---|---|---|---|
| GTIN | 08714729370154 | LOT | 12345678 |
| REF Catalog No. | H749389282015 0 | Use By | 2010-12-31 |

STERILE EO Sterilized using ethylene oxide.

90244533-01

Internal BSC Bar Code

92425134-29A

CE 0344

**Made in MALAYSIA**
PMT 741, Persiaran Cassia Selatan 1
Taman Perindustrian Batu Kawan
14110 Bandar Cassia,
Pulau Pinang, MALAYSIA

Boston Scientific
Maverick²™
1.5mm x 20mm
GTIN 08714729370154
REF H7493892820150
LOT 12345678

Boston Scientific
Maverick²™
1.5mm x 20mm
GTIN 08714729370154
REF H7493892820150
LOT 12345678

(01)08714729370154(17)101231(10)12345678 GS1

This product may be protected by one or more patents. Patent information can be obtained at http://www.bostonscientific.com/patents

**Label Specification Part Number:92425134-29A**

Boston Scientific

**2.0mm x 20mm**

# Maverick²™

## MONORAIL™


### PTCA Dilatation Catheter

Catéter de dilatación para ACTP, Cathéter de dilatation pour ACTP, PTCA-Dilatationskatheter, Catetere dilatatore per PTCA, PTCA dilatatiekatheter, PTCA拡張カテーテル, PTCA-dilatationskateter, Καθετήρας διαστολής PTCA, Cateter de Dilatação para PTCA, PTCA-dilatationskateter, PTCA-tágítókatéter, Dilatační katétr pro PTCA, Cewnik rozszerzający do PTCA, PTCA-dilatasjonskateter, PTKA Dilatasyon Kateteri

| atm - kPa Pressure | | 2.0mm Balloon O.D. |
|---|---|---|
| 5.0 - 507 | | 1.97 |
| 6.0 - 608 | NOMINAL | 2.00 |
| 7.0 - 709 | | 2.03 |
| 8.0 - 811 | | 2.06 |
| 9.0 - 912 | | 2.09 |
| 10.0 - 1013 | | 2.12 |
| 11.0 - 1115 | | 2.15 |
| 12.0 - 1216 | RATED* | 2.19 |
| 13.0 - 1317 | | -- |
| 14.0 - 1419 | | -- |

*Rated Burst Pressure. DO NOT EXCEED.

Contents (1)




CL (1) Includes CLIPIT™ Hypotube Clip

GW R 0.014in (≤0.36mm) Recommended Guidewire

GC R 5F (≥0.058in/1.47mm) Recommended Guide Catheter

| | | | |
|---|---|---|---|
| **GTIN** | 08714729370161 | LOT | 12345678 |
| REF Catalog No. | H749389282020o | Use By | 2010-12-31 |

STERILE EO Sterilized using ethylene oxide.

90244533-01

Internal BSC Bar Code

92425134-30A

CE 0344

**Made in MALAYSIA**
PMT 741, Persiaran Cassia Selatan 1
Taman Perindustrian Batu Kawan
14110 Bandar Cassia,
Pulau Pinang, MALAYSIA

Boston Scientific
Maverick²™
2.0mm x 20mm
GTIN 08714729370161
REF H7493892820200
LOT 12345678

Boston Scientific
Maverick²™
2.0mm x 20mm
GTIN 08714729370161
REF H7493892820200
LOT 12345678

(01)08714729370161(17)101231(10)12345678 GS1

This product may be protected by one or more patents. Patent information can be obtained at http://www.bostonscientific.com/patents

**Label Specification Part Number:92425134-30A**

Boston Scientific

**2.25mm x 20mm**

# Maverick²™

## MONORAIL™


### PTCA Dilatation Catheter

Catéter de dilatación para ACTP, Cathéter de dilatation pour ACTP, PTCA-Dilatationskatheter, Catetere dilatatore per PTCA, PTCA dilatatiekatheter, PTCA拡張カテーテル, PTCA-dilatationskateter, Καθετήρας διαστολής PTCA, Cateter de Dilatação para PTCA, PTCA-dilatationskateter, PTCA-tágítókatéter, Dilatační katétr pro PTCA, Cewnik rozszerzający do PTCA, PTCA-dilatasjonskateter, PTKA Dilatasyon Kateteri

| atm - kPa Pressure | | 2.25mm Balloon O.D. |
|---|---|---|
| 5.0 - 507 | | 2.22 |
| 6.0 - 608 | NOMINAL | 2.25 |
| 7.0 - 709 | | 2.28 |
| 8.0 - 811 | | 2.31 |
| 9.0 - 912 | | 2.35 |
| 10.0 - 1013 | | 2.38 |
| 11.0 - 1115 | | 2.41 |
| 12.0 - 1216 | | 2.44 |
| 13.0 - 1317 | | 2.47 |
| 14.0 - 1419 | RATED* | 2.51 |

*Rated Burst Pressure and Stent Rated Burst Pressure. DO NOT EXCEED.

Contents (1)




CL (1) Includes CLIPIT™ Hypotube Clip

GW R 0.014in (≤0.36mm) Recommended Guidewire

GC R 5F (≥0.058in/1.47mm) Recommended Guide Catheter

| | | | |
|---|---|---|---|
| **GTIN** | 08714729370178 | LOT | 12345678 |
| REF Catalog No. | H749389282022o | Use By | 2010-12-31 |

STERILE EO Sterilized using ethylene oxide.

90244533-01

Internal BSC Bar Code

92425134-31A

Boston Scientific
Maverick²™
2.25mm x 20mm
GTIN 08714729370178
REF H7493892820220
LOT 12345678

Boston Scientific
Maverick²™
2.25mm x 20mm
GTIN 08714729370178
REF H7493892820220
LOT 12345678

(01)08714729370178(17)101231(10)12345678 GS1

CE 0344

**Made in MALAYSIA**
PMT 741, Persiaran Cassia Selatan 1
Taman Perindustrian Batu Kawan
14110 Bandar Cassia,
Pulau Pinang, MALAYSIA

This product may be protected by one or more patents. Patent information can be obtained at http://www.bostonscientific.com/patents

**Label Specification Part Number:92425134-31A**

Boston Scientific

2.5mm x 20mm

# Maverick²™

## MONORAIL™


### PTCA Dilatation Catheter

Catéter de dilatación para ACTP, Cathéter de dilatation pour ACTP, PTCA-Dilatationskatheter, Catetere dilatatore per PTCA, PTCA dilatatiekatheter, PTCA拡張カテーテル, PTCA-dilatationskateter, Καθετήρας διαστολής PTCA, Cateter de Dilatação para PTCA, PTCA-dilatationskateter, PTCA-tágítókatéter, Dilatační katétr pro PTCA, Cewnik rozszerzający do PTCA, PTCA-dilatasjonskateter, PTKA Dilatasyon Kateteri

| atm - kPa Pressure | | 2.5mm Balloon O.D. |
|---|---|---|
| 5.0 - 507 | | 2.46 |
| 6.0 - 608 | NOMINAL | 2.50 |
| 7.0 - 709 | | 2.54 |
| 8.0 - 811 | | 2.58 |
| 9.0 - 912 | | 2.62 |
| 10.0 - 1013 | | 2.67 |
| 11.0 - 1115 | | 2.71 |
| 12.0 - 1216 | | 2.75 |
| 13.0 - 1317 | | 2.79 |
| 14.0 - 1419 | RATED* | 2.83 |

*Rated Burst Pressure and Stent Rated Burst Pressure. DO NOT EXCEED.

Contents (1)




CL (1) Includes CLIPIT™ Hypotube Clip

GW R 0.014in (≤0.36mm) Recommended Guidewire

GC R 5F (≥0.058in/1.47mm) Recommended Guide Catheter

| | | | |
|---|---|---|---|
| **GTIN** | 08714729370185 | LOT | 12345678 |
| REF Catalog No. | H749389282025O | Use By | 2010-12-31 |

STERILE EO Sterilized using ethylene oxide.

90244533-01

Internal BSC Bar Code

92425134-32A

Boston Scientific
Maverick²™
2.5mm x 20mm
GTIN 08714729370185
REF H7493892820250
LOT 12345678

Boston Scientific
Maverick²™
2.5mm x 20mm
GTIN 08714729370185
REF H7493892820250
LOT 12345678

CE 0344

(01)08714729370185(17)101231(10)12345678 GS1

**Made in MALAYSIA**
PMT 741, Persiaran Cassia Selatan 1
Taman Perindustrian Batu Kawan
14110 Bandar Cassia,
Pulau Pinang, MALAYSIA

This product may be protected by one or more patents. Patent information can be obtained at http://www.bostonscientific.com/patents

**Label Specification Part Number:92425134-32A**

Boston Scientific

2.75mm x20mm

# Maverick²™

## MONORAIL™


### PTCA Dilatation Catheter

Catéter de dilatación para ACTP, Cathéter de dilatation pour ACTP, PTCA-Dilatationskatheter, Catetere dilatatore per PTCA, PTCA dilatatiekatheter, PTCA拡張カテーテル, PTCA-dilatationskateter, Καθετήρας διαστολής PTCA, Cateter de Dilatação para PTCA, PTCA-dilatationskateter, PTCA-tágítókatéter, Dilatační katétr pro PTCA, Cewnik rozszerzający do PTCA, PTCA-dilatasjonskateter, PTKA Dilatasyon Kateteri

| atm - kPa Pressure | | 2.75mm Balloon O.D. |
|---|---|---|
| 5.0 - 507 | | 2.71 |
| 6.0 - 608 | NOMINAL | 2.75 |
| 7.0 - 709 | | 2.79 |
| 8.0 - 811 | | 2.83 |
| 9.0 - 912 | | 2.87 |
| 10.0 - 1013 | | 2.91 |
| 11.0 - 1115 | | 2.95 |
| 12.0 - 1216 | | 2.99 |
| 13.0 - 1317 | | 3.03 |
| 14.0 - 1419 | RATED* | 3.07 |

*Rated Burst Pressure and Stent Rated Burst Pressure. DO NOT EXCEED.

Contents (1)




CL (1) Includes CLIPIT™ Hypotube Clip

GW R 0.014in (≤0.36mm) Recommended Guidewire

GC R 5F (≥0.058in/1.47mm) Recommended Guide Catheter

| | | | |
|---|---|---|---|
| GTIN | 08714729370192 | LOT | 12345678 |
| REF Catalog No. | H749389282027o | Use By | 2010-12-31 |

STERILE EO Sterilized using ethylene oxide.

90244533-01

Internal BSC Bar Code

92425134-33A

Boston Scientific
Maverick²™
2.75mm x 20mm
GTIN 08714729370192
REF H7493892820270
LOT 12345678

Boston Scientific
Maverick²™
2.75mm x 20mm
GTIN 08714729370192
REF H7493892820270
LOT 12345678

CE 0344

(01)08714729370192(17)101231(10)12345678 GS1

**Made in MALAYSIA**
PMT 741, Persiaran Cassia Selatan 1
Taman Perindustrian Batu Kawan
14110 Bandar Cassia,
Pulau Pinang, MALAYSIA

This product may be protected by one or more patents. Patent information can be obtained at http://www.bostonscientific.com/patents

**Label Specification Part Number:92425134-33A**

Boston Scientific

**3.0mm x 20mm**

# Maverick²™

## MONORAIL™


### PTCA Dilatation Catheter

Catéter de dilatación para ACTP, Cathéter de dilatation pour ACTP, PTCA-Dilatationskatheter, Catetere dilatatore per PTCA, PTCA dilatatiekatheter, PTCA拡張カテーテル, PTCA-dilatationskateter, Καθετήρας διαστολής PTCA, Cateter de Dilatação para PTCA, PTCA-dilatationskateter, PTCA-tágítókatéter, Dilatační katétr pro PTCA, Cewnik rozszerzający do PTCA, PTCA-dilatasjonskateter, PTKA Dilatasyon Kateteri

| atm - kPa Pressure | | 3.0mm Balloon O.D. |
|---|---|---|
| 5.0 - 507 | | 2.95 |
| 6.0 - 608 | NOMINAL | 3.00 |
| 7.0 - 709 | | 3.05 |
| 8.0 - 811 | | 3.09 |
| 9.0 - 912 | | 3.14 |
| 10.0 - 1013 | | 3.18 |
| 11.0 - 1115 | | 3.23 |
| 12.0 - 1216 | | 3.28 |
| 13.0 - 1317 | | 3.32 |
| 14.0 - 1419 | RATED* | 3.37 |

*Rated Burst Pressure and Stent Rated Burst Pressure. DO NOT EXCEED.

Contents (1)




CL (1) Includes CLIPIT™ Hypotube Clip

GW R 0.014in (≤0.36mm) Recommended Guidewire

GC R 5F (≥0.058in/1.47mm) Recommended Guide Catheter

| | | | |
|---|---|---|---|
| **GTIN** | 08714729370208 | LOT | 12345678 |
| REF Catalog No. | H749389282030o | Use By | 2010-12-31 |

STERILE EO Sterilized using ethylene oxide.

90244533-01

Internal BSC Bar Code

92425134-34A

CE 0344

**Made in MALAYSIA**
PMT 741, Persiaran Cassia Selatan 1
Taman Perindustrian Batu Kawan
14110 Bandar Cassia,
Pulau Pinang, MALAYSIA

Boston Scientific
Maverick²™
3.0mm x 20mm
GTIN 08714729370208
REF H7493892820300
LOT 12345678

Boston Scientific
Maverick²™
3.0mm x 20mm
GTIN 08714729370208
REF H7493892820300
LOT 12345678

(01)08714729370208(17)101231(10)12345678 GS1

This product may be protected by one or more patents. Patent information can be obtained at http://www.bostonscientific.com/patents

**Label Specification Part Number:92425134-34A**

Boston Scientific

3.25mm x 20mm

# Maverick²™

## MONORAIL™


### PTCA Dilatation Catheter

Catéter de dilatación para ACTP, Cathéter de dilatation pour ACTP, PTCA-Dilatationskatheter, Catetere dilatatore per PTCA, PTCA dilatatiekatheter, PTCA拡張カテーテル, PTCA-dilatationskateter, Καθετήρας διαστολής PTCA, Cateter de Dilatação para PTCA, PTCA-dilatationskateter, PTCA-tágítókatéter, Dilatační katétr pro PTCA, Cewnik rozszerzający do PTCA, PTCA-dilatasjonskateter, PTKA Dilatasyon Kateteri

| atm - kPa Pressure | | 3.25mm Balloon O.D. |
|---|---|---|
| 5.0 - 507 | | 3.20 |
| 6.0 - 608 | NOMINAL | 3.25 |
| 7.0 - 709 | | 3.30 |
| 8.0 - 811 | | 3.34 |
| 9.0 - 912 | | 3.39 |
| 10.0 - 1013 | | 3.43 |
| 11.0 - 1115 | | 3.48 |
| 12.0 - 1216 | | 3.52 |
| 13.0 - 1317 | | 3.57 |
| 14.0 - 1419 | RATED* | 3.61 |

*Rated Burst Pressure and Stent Rated Burst Pressure. DO NOT EXCEED.

Contents (1)




CL (1) Includes CLIPIT™ Hypotube Clip

GW R 0.014in (≤0.36mm) Recommended Guidewire

GC R 5F (≥0.058in/1.47mm) Recommended Guide Catheter

| | | | |
|---|---|---|---|
| **GTIN** | 08714729370215 | LOT | 12345678 |
| REF Catalog No. | H749389282032o | Use By | 2010-12-31 |

STERILE EO Sterilized using ethylene oxide.

90244533-01

Internal BSC Bar Code

92425134-35A

CE 0344

**Made in MALAYSIA**
PMT 741, Persiaran Cassia Selatan 1
Taman Perindustrian Batu Kawan
14110 Bandar Cassia,
Pulau Pinang, MALAYSIA

Boston Scientific
Maverick²™
3.25mm x 20mm
GTIN 08714729370215
REF H7493892820320
LOT 12345678

Boston Scientific
Maverick²™
3.25mm x 20mm
GTIN 08714729370215
REF H7493892820320
LOT 12345678

(01)08714729370215(17)101231(10)12345678 GS1

This product may be protected by one or more patents. Patent information can be obtained at http://www.bostonscientific.com/patents

**Label Specification Part Number:92425134-35A**

Boston Scientific

3.5mm x 20mm

# Maverick²™

## MONORAIL™


### PTCA Dilatation Catheter

Catéter de dilatación para ACTP, Cathéter de dilatation pour ACTP, PTCA-Dilatationskatheter, Catetere dilatatore per PTCA, PTCA dilatatiekatheter, PTCA拡張カテーテル, PTCA-dilatationskateter, Καθετήρας διαστολής PTCA, Cateter de Dilatação para PTCA, PTCA-dilatationskateter, PTCA-tágítókatéter, Dilatační katétr pro PTCA, Cewnik rozszerzający do PTCA, PTCA-dilatasjonskateter, PTKA Dilatasyon Kateteri

| atm - kPa Pressure | | 3.5mm Balloon O.D. |
|---|---|---|
| 5.0 - 507 | | 3.45 |
| 6.0 - 608 | NOMINAL | 3.50 |
| 7.0 - 709 | | 3.55 |
| 8.0 - 811 | | 3.60 |
| 9.0 - 912 | | 3.65 |
| 10.0 - 1013 | | 3.71 |
| 11.0 - 1115 | | 3.76 |
| 12.0 - 1216 | RATED* | 3.81 |
| 13.0 - 1317 | | -- |
| 14.0 - 1419 | | -- |

*Rated Burst Pressure and Stent Rated Burst Pressure. DO NOT EXCEED.

Contents (1)




CL (1) Includes CLIPIT™ Hypotube Clip

GW R 0.014in (≤0.36mm) Recommended Guidewire

GC R 5F (≥0.058in/1.47mm) Recommended Guide Catheter

| | | | |
|---|---|---|---|
| **GTIN** | 08714729370222 | LOT | 12345678 |
| REF Catalog No. | H749389282035O | Use By | 2010-12-31 |

STERILE EO Sterilized using ethylene oxide.

90244533-01

Internal BSC Bar Code

92425134-36A

CE 0344

**Made in MALAYSIA**
PMT 741, Persiaran Cassia Selatan 1
Taman Perindustrian Batu Kawan
14110 Bandar Cassia,
Pulau Pinang, MALAYSIA

Boston Scientific
Maverick²™
3.5mm x 20mm
GTIN 08714729370222
REF H7493892820350
LOT 12345678

Boston Scientific
Maverick²™
3.5mm x 20mm
GTIN 08714729370222
REF H7493892820350
LOT 12345678

(01)08714729370222(17)101231(10)12345678 GS1

This product may be protected by one or more patents. Patent information can be obtained at http://www.bostonscientific.com/patents

**Label Specification Part Number:92425134-36A**

Boston Scientific

3.75mm x20mm

# Maverick²™

## MONORAIL™


### PTCA Dilatation Catheter

Catéter de dilatación para ACTP, Cathéter de dilatation pour ACTP, PTCA-Dilatationskatheter, Catetere dilatatore per PTCA, PTCA dilatatiekatheter, PTCA拡張カテーテル, PTCA-dilatationskateter, Καθετήρας διαστολής PTCA, Cateter de Dilatação para PTCA, PTCA-dilatationskateter, PTCA-tágítókatéter, Dilatační katétr pro PTCA, Cewnik rozszerzający do PTCA, PTCA-dilatasjonskateter, PTKA Dilatasyon Kateteri

| atm - kPa Pressure | | 3.75mm Balloon O.D. |
|---|---|---|
| 5.0 - 507 | | 3.70 |
| 6.0 - 608 | NOMINAL | 3.75 |
| 7.0 - 709 | | 3.80 |
| 8.0 - 811 | | 3.85 |
| 9.0 - 912 | | 3.90 |
| 10.0 - 1013 | | 3.95 |
| 11.0 - 1115 | | 4.00 |
| 12.0 - 1216 | RATED* | 4.05 |
| 13.0 - 1317 | | -- |
| 14.0 - 1419 | | -- |

*Rated Burst Pressure and Stent Rated Burst Pressure. DO NOT EXCEED.

Contents (1)




CL (1) Includes CLIPIT™ Hypotube Clip

GW R 0.014in (≤0.36mm) Recommended Guidewire

GC R 5F (≥0.058in/1.47mm) Recommended Guide Catheter

| | | | |
|---|---|---|---|
| GTIN | 08714729370239 | LOT | 12345678 |
| REF Catalog No. | H749389282037o | Use By | 2010-12-31 |

STERILE EO Sterilized using ethylene oxide.

90244533-01

Internal BSC Bar Code

92425134-37A

CE 0344

**Made in MALAYSIA**
PMT 741, Persiaran Cassia Selatan 1
Taman Perindustrian Batu Kawan
14110 Bandar Cassia,
Pulau Pinang, MALAYSIA

Boston Scientific
Maverick²™
3.75mm x 20mm
GTIN 08714729370239
REF H7493892820370
LOT 12345678

Boston Scientific
Maverick²™
3.75mm x 20mm
GTIN 08714729370239
REF H7493892820370
LOT 12345678

(01)08714729370239(17)101231(10)12345678 GS1

This product may be protected by one or more patents. Patent information can be obtained at http://www.bostonscientific.com/patents

**Label Specification Part Number:92425134-37A**

Boston Scientific

**4.0mm x 20mm**

# Maverick²™

## MONORAIL™


### PTCA Dilatation Catheter

Catéter de dilatación para ACTP, Cathéter de dilatation pour ACTP, PTCA-Dilatationskatheter, Catetere dilatatore per PTCA, PTCA dilatatiekatheter, PTCA拡張カテーテル, PTCA-dilatationskateter, Καθετήρας διαστολής PTCA, Cateter de Dilatação para PTCA, PTCA-dilatationskateter, PTCA-tágítókatéter, Dilatační katétr pro PTCA, Cewnik rozszerzający do PTCA, PTCA-dilatasjonskateter, PTKA Dilatasyon Kateteri

| atm - kPa Pressure | | 4.0mm Balloon O.D. |
|---|---|---|
| 5.0 - 507 | | 3.95 |
| 6.0 - 608 | NOMINAL | 4.00 |
| 7.0 - 709 | | 4.05 |
| 8.0 - 811 | | 4.10 |
| 9.0 - 912 | | 4.15 |
| 10.0 - 1013 | | 4.20 |
| 11.0 - 1115 | | 4.25 |
| 12.0 - 1216 | RATED* | 4.31 |
| 13.0 - 1317 | | -- |
| 14.0 - 1419 | | -- |

*Rated Burst Pressure and Stent Rated Burst Pressure. DO NOT EXCEED.

Contents (1)




CL (1) Includes CLIPIT™ Hypotube Clip

GW R 0.014in (≤0.36mm) Recommended Guidewire

GC R 5F (≥0.058in/1.47mm) Recommended Guide Catheter

| | | | |
|---|---|---|---|
| **GTIN** | 08714729370246 | LOT | 12345678 |
| REF Catalog No. | H749389282040o | Use By | 2010-12-31 |

STERILE EO Sterilized using ethylene oxide.

90244533-01

Internal BSC Bar Code

92425134-38A

CE 0344

**Made in MALAYSIA**
PMT 741, Persiaran Cassia Selatan 1
Taman Perindustrian Batu Kawan
14110 Bandar Cassia,
Pulau Pinang, MALAYSIA

Boston Scientific
Maverick²™
4.0mm x 20mm
GTIN 08714729370246
REF H7493892820400
LOT 12345678

Boston Scientific
Maverick²™
4.0mm x 20mm
GTIN 08714729370246
REF H7493892820400
LOT 12345678

(01)08714729370246(17)101231(10)12345678 GS1

This product may be protected by one or more patents. Patent information can be obtained at http://www.bostonscientific.com/patents

**Label Specification Part Number:92425134-38A**

Boston Scientific

**2.0mm x 25mm**

# Maverick²™

## MONORAIL™


### PTCA Dilatation Catheter

Catéter de dilatación para ACTP, Cathéter de dilatation pour ACTP, PTCA-Dilatationskatheter, Catetere dilatatore per PTCA, PTCA dilatatiekatheter, PTCA拡張カテーテル, PTCA-dilatationskateter, Καθετήρας διαστολής PTCA, Cateter de Dilatação para PTCA, PTCA-dilatationskateter, PTCA-tágítókatéter, Dilatační katétr pro PTCA, Cewnik rozszerzający do PTCA, PTCA-dilatasjonskateter, PTKA Dilatasyon Kateteri

| atm - kPa Pressure | | 2.0mm Balloon O.D. |
|---|---|---|
| 5.0 - 507 | | 1.97 |
| 6.0 - 608 | NOMINAL | 2.00 |
| 7.0 - 709 | | 2.03 |
| 8.0 - 811 | | 2.06 |
| 9.0 - 912 | | 2.09 |
| 10.0 - 1013 | | 2.12 |
| 11.0 - 1115 | | 2.15 |
| 12.0 - 1216 | RATED* | 2.19 |
| 13.0 - 1317 | | -- |
| 14.0 - 1419 | | -- |

*Rated Burst Pressure. DO NOT EXCEED.

Contents (1)




CL (1) Includes CLIPIT™ Hypotube Clip

GW R 0.014in (≤0.36mm) Recommended Guidewire

GC R 5F (≥0.058in/1.47mm) Recommended Guide Catheter

| | | | |
|---|---|---|---|
| **GTIN** | 08714729370253 | LOT | 12345678 |
| REF Catalog No. | H749389282520 0 | Use By | 2010-12-31 |

STERILE EO Sterilized using ethylene oxide.

90244533-01

Internal BSC Bar Code

92425134-39A

CE 0344

**Made in MALAYSIA**
PMT 741, Persiaran Cassia Selatan 1
Taman Perindustrian Batu Kawan
14110 Bandar Cassia,
Pulau Pinang, MALAYSIA

Boston Scientific
Maverick²™
2.0mm x 25mm
GTIN 08714729370253
REF H7493892825200
LOT 12345678

Boston Scientific
Maverick²™
2.0mm x 25mm
GTIN 08714729370253
REF H7493892825200
LOT 12345678

(01)08714729370253(17)101231(10)12345678 GS1

This product may be protected by one or more patents. Patent information can be obtained at http://www.bostonscientific.com/patents

**Label Specification Part Number:92425134-39A**

Boston Scientific

2.25mm x25mm

# Maverick²™

## MONORAIL™


### PTCA Dilatation Catheter

Catéter de dilatación para ACTP, Cathéter de dilatation pour ACTP, PTCA-Dilatationskatheter, Catetere dilatatore per PTCA, PTCA dilatatiekatheter, PTCA拡張カテーテル, PTCA-dilatationskateter, Καθετήρας διαστολής PTCA, Cateter de Dilatação para PTCA, PTCA-dilatationskateter, PTCA-tágítókatéter, Dilatační katétr pro PTCA, Cewnik rozszerzający do PTCA, PTCA-dilatasjonskateter, PTKA Dilatasyon Kateteri

| atm - kPa Pressure | | 2.25mm Balloon O.D. |
|---|---|---|
| 5.0 - 507 | | 2.22 |
| 6.0 - 608 | NOMINAL | 2.25 |
| 7.0 - 709 | | 2.28 |
| 8.0 - 811 | | 2.31 |
| 9.0 - 912 | | 2.35 |
| 10.0 - 1013 | | 2.38 |
| 11.0 - 1115 | | 2.41 |
| 12.0 - 1216 | | 2.44 |
| 13.0 - 1317 | | 2.47 |
| 14.0 - 1419 | RATED* | 2.51 |

*Rated Burst Pressure and Stent Rated Burst Pressure. DO NOT EXCEED.

Contents (1)




CL (1) Includes CLIPIT™ Hypotube Clip

GW R 0.014in (≤0.36mm) Recommended Guidewire

GC R 5F (≥0.058in/1.47mm) Recommended Guide Catheter

| | | | |
|---|---|---|---|
| GTIN | 08714729370260 | LOT | 12345678 |
| REF Catalog No. | H749389282522o | Use By | 2010-12-31 |

STERILE EO Sterilized using ethylene oxide.

90244533-01

Internal BSC Bar Code

92425134-40A

CE 0344

**Made in MALAYSIA**
PMT 741, Persiaran Cassia Selatan 1
Taman Perindustrian Batu Kawan
14110 Bandar Cassia,
Pulau Pinang, MALAYSIA

Boston Scientific
Maverick²™
2.25mm x 25mm
GTIN 08714729370260
REF H7493892825220
LOT 12345678

Boston Scientific
Maverick²™
2.25mm x 25mm
GTIN 08714729370260
REF H7493892825220
LOT 12345678

(01)08714729370260(17)101231(10)12345678 GS1

This product may be protected by one or more patents. Patent information can be obtained at http://www.bostonscientific.com/patents

**Label Specification Part Number:92425134-40A**

Boston Scientific

**2.5mm x 25mm**

# Maverick²™

## MONORAIL™


### PTCA Dilatation Catheter

Catéter de dilatación para ACTP, Cathéter de dilatation pour ACTP, PTCA-Dilatationskatheter, Catetere dilatatore per PTCA, PTCA dilatatiekatheter, PTCA拡張カテーテル, PTCA-dilatationskateter, Καθετήρας διαστολής PTCA, Cateter de Dilatação para PTCA, PTCA-dilatationskateter, PTCA-tágítókatéter, Dilatační katétr pro PTCA, Cewnik rozszerzający do PTCA, PTCA-dilatasjonskateter, PTKA Dilatasyon Kateteri

| atm - kPa Pressure | | 2.5mm Balloon O.D. |
|---|---|---|
| 5.0 - 507 | | 2.46 |
| 6.0 - 608 | NOMINAL | 2.50 |
| 7.0 - 709 | | 2.54 |
| 8.0 - 811 | | 2.58 |
| 9.0 - 912 | | 2.62 |
| 10.0 - 1013 | | 2.67 |
| 11.0 - 1115 | | 2.71 |
| 12.0 - 1216 | | 2.75 |
| 13.0 - 1317 | | 2.79 |
| 14.0 - 1419 | RATED* | 2.83 |

*Rated Burst Pressure and Stent Rated Burst Pressure. DO NOT EXCEED.

Contents (1)




CL (1) Includes CLIPIT™ Hypotube Clip

GW R 0.014in (≤0.36mm) Recommended Guidewire

GC R 5F (≥0.058in/1.47mm) Recommended Guide Catheter

| | | | |
|---|---|---|---|
| **GTIN** | 08714729370277 | LOT | 12345678 |
| REF Catalog No. | H749389282525O | Use By | 2010-12-31 |

STERILE EO Sterilized using ethylene oxide.

90244533-01

Internal BSC Bar Code

92425134-41A

Boston Scientific
Maverick²™
2.5mm x 25mm
GTIN 08714729370277
REF H7493892825250
LOT 12345678

Boston Scientific
Maverick²™
2.5mm x 25mm
GTIN 08714729370277
REF H7493892825250
LOT 12345678

CE 0344

(01)08714729370277(17)101231(10)12345678 GS1

**Made in MALAYSIA**
PMT 741, Persiaran Cassia Selatan 1
Taman Perindustrian Batu Kawan
14110 Bandar Cassia,
Pulau Pinang, MALAYSIA

This product may be protected by one or more patents. Patent information can be obtained at http://www.bostonscientific.com/patents

**Label Specification Part Number:92425134-41A**

Boston Scientific

2.75mm x25mm

# Maverick²™

## MONORAIL™


### PTCA Dilatation Catheter

Catéter de dilatación para ACTP, Cathéter de dilatation pour ACTP, PTCA-Dilatationskatheter, Catetere dilatatore per PTCA, PTCA dilatatiekatheter, PTCA拡張カテーテル, PTCA-dilatationskateter, Καθετήρας διαστολής PTCA, Cateter de Dilatação para PTCA, PTCA-dilatationskateter, PTCA-tágítókatéter, Dilatační katétr pro PTCA, Cewnik rozszerzający do PTCA, PTCA-dilatasjonskateter, PTKA Dilatasyon Kateteri

| atm - kPa Pressure | | 2.75mm Balloon O.D. |
|---|---|---|
| 5.0 - 507 | | 2.71 |
| 6.0 - 608 | NOMINAL | 2.75 |
| 7.0 - 709 | | 2.79 |
| 8.0 - 811 | | 2.83 |
| 9.0 - 912 | | 2.87 |
| 10.0 - 1013 | | 2.91 |
| 11.0 - 1115 | | 2.95 |
| 12.0 - 1216 | | 2.99 |
| 13.0 - 1317 | | 3.03 |
| 14.0 - 1419 | RATED* | 3.07 |

*Rated Burst Pressure and Stent Rated Burst Pressure. DO NOT EXCEED.

Contents (1)




CL (1) Includes CLIPIT™ Hypotube Clip

GW R 0.014in (≤0.36mm) Recommended Guidewire

GC R 5F (≥0.058in/1.47mm) Recommended Guide Catheter

| | | | |
|---|---|---|---|
| **GTIN** | 08714729370284 | LOT | 12345678 |
| REF Catalog No. | H749389282527o | Use By | 2010-12-31 |

STERILE EO Sterilized using ethylene oxide.

90244533-01

Internal BSC Bar Code

92425134-42A

Boston Scientific
Maverick²™
2.75mm x 25mm
GTIN 08714729370284
REF H7493892825270
LOT 12345678

Boston Scientific
Maverick²™
2.75mm x 25mm
GTIN 08714729370284
REF H7493892825270
LOT 12345678

(01)08714729370284(17)101231(10)12345678 GS1

CE 0344

**Made in MALAYSIA**
PMT 741, Persiaran Cassia Selatan 1
Taman Perindustrian Batu Kawan
14110 Bandar Cassia,
Pulau Pinang, MALAYSIA

This product may be protected by one or more patents. Patent information can be obtained at http://www.bostonscientific.com/patents

**Label Specification Part Number:92425134-42A**

Boston Scientific

**3.0mm x 25mm**

# Maverick²™

## MONORAIL™


### PTCA Dilatation Catheter

Catéter de dilatación para ACTP, Cathéter de dilatation pour ACTP, PTCA-Dilatationskatheter, Catetere dilatatore per PTCA, PTCA dilatatiekatheter, PTCA拡張カテーテル, PTCA-dilatationskateter, Καθετήρας διαστολής PTCA, Cateter de Dilatação para PTCA, PTCA-dilatationskateter, PTCA-tágítókatéter, Dilatační katétr pro PTCA, Cewnik rozszerzający do PTCA, PTCA-dilatasjonskateter, PTKA Dilatasyon Kateteri

| atm - kPa Pressure | | 3.0mm Balloon O.D. |
|---|---|---|
| 5.0 - 507 | | 2.95 |
| 6.0 - 608 | NOMINAL | 3.00 |
| 7.0 - 709 | | 3.05 |
| 8.0 - 811 | | 3.09 |
| 9.0 - 912 | | 3.14 |
| 10.0 - 1013 | | 3.18 |
| 11.0 - 1115 | | 3.23 |
| 12.0 - 1216 | | 3.28 |
| 13.0 - 1317 | | 3.32 |
| 14.0 - 1419 | RATED* | 3.37 |

*Rated Burst Pressure and Stent Rated Burst Pressure. DO NOT EXCEED.

Contents (1)




CL (1) Includes CLIPIT™ Hypotube Clip

GW R 0.014in (≤0.36mm) Recommended Guidewire

GC R 5F (≥0.058in/1.47mm) Recommended Guide Catheter

| | | | |
|---|---|---|---|
| **GTIN** | 08714729370291 | LOT | 12345678 |
| REF Catalog No. | H749389282530 0 | Use By | 2010-12-31 |

STERILE EO Sterilized using ethylene oxide.

90244533-01

Internal BSC Bar Code

92425134-43A

Boston Scientific
Maverick²™
3.0mm x 25mm
GTIN 08714729370291
REF H7493892825300
LOT 12345678

Boston Scientific
Maverick²™
3.0mm x 25mm
GTIN 08714729370291
REF H7493892825300
LOT 12345678

CE 0344

(01)08714729370291(17)101231(10)12345678 GS1

**Made in MALAYSIA**
PMT 741, Persiaran Cassia Selatan 1
Taman Perindustrian Batu Kawan
14110 Bandar Cassia,
Pulau Pinang, MALAYSIA

This product may be protected by one or more patents. Patent information can be obtained at http://www.bostonscientific.com/patents

**Label Specification Part Number:92425134-43A**

Boston Scientific

3.25mm x25mm

# Maverick²™

## MONORAIL™


### PTCA Dilatation Catheter

Catéter de dilatación para ACTP, Cathéter de dilatation pour ACTP, PTCA-Dilatationskatheter, Catetere dilatatore per PTCA, PTCA dilatatiekatheter, PTCA拡張カテーテル, PTCA-dilatationskateter, Καθετήρας διαστολής PTCA, Cateter de Dilatação para PTCA, PTCA-dilatationskateter, PTCA-tágítókatéter, Dilatační katétr pro PTCA, Cewnik rozszerzający do PTCA, PTCA-dilatasjonskateter, PTKA Dilatasyon Kateteri

| atm - kPa Pressure | | 3.25mm Balloon O.D. |
|---|---|---|
| 5.0 - 507 | | 3.20 |
| 6.0 - 608 | NOMINAL | 3.25 |
| 7.0 - 709 | | 3.30 |
| 8.0 - 811 | | 3.34 |
| 9.0 - 912 | | 3.39 |
| 10.0 - 1013 | | 3.43 |
| 11.0 - 1115 | | 3.48 |
| 12.0 - 1216 | | 3.52 |
| 13.0 - 1317 | | 3.57 |
| 14.0 - 1419 | RATED* | 3.61 |

*Rated Burst Pressure and Stent Rated Burst Pressure. DO NOT EXCEED.

Contents (1)




CL (1) Includes CLIPIT™ Hypotube Clip

GW R 0.014in (≤0.36mm) Recommended Guidewire

GC R 5F (≥0.058in/1.47mm) Recommended Guide Catheter

| | | | |
|---|---|---|---|
| **GTIN** | 08714729370307 | LOT | 12345678 |
| REF Catalog No. | H749389282532o | Use By | 2010-12-31 |

STERILE EO Sterilized using ethylene oxide.

90244533-01

Internal BSC Bar Code

92425134-44A

Boston Scientific
Maverick²™
3.25mm x 25mm
GTIN 08714729370307
REF H7493892825320
LOT 12345678

Boston Scientific
Maverick²™
3.25mm x 25mm
GTIN 08714729370307
REF H7493892825320
LOT 12345678

CE 0344

(01)08714729370307(17)101231(10)12345678 GS1

**Made in MALAYSIA**
PMT 741, Persiaran Cassia Selatan 1
Taman Perindustrian Batu Kawan
14110 Bandar Cassia,
Pulau Pinang, MALAYSIA

This product may be protected by one or more patents. Patent information can be obtained at http://www.bostonscientific.com/patents

**Label Specification Part Number:92425134-44A**

Boston Scientific

3.5mm x 25mm

# Maverick²™

## MONORAIL™


### PTCA Dilatation Catheter

Catéter de dilatación para ACTP, Cathéter de dilatation pour ACTP, PTCA-Dilatationskatheter, Catetere dilatatore per PTCA, PTCA dilatatiekatheter, PTCA拡張カテーテル, PTCA-dilatationskateter, Καθετήρας διαστολής PTCA, Cateter de Dilatação para PTCA, PTCA-dilatationskateter, PTCA-tágítókatéter, Dilatační katétr pro PTCA, Cewnik rozszerzający do PTCA, PTCA-dilatasjonskateter, PTKA Dilatasyon Kateteri

| atm - kPa Pressure | | 3.5mm Balloon O.D. |
|---|---|---|
| 5.0 - 507 | | 3.45 |
| 6.0 - 608 | NOMINAL | 3.50 |
| 7.0 - 709 | | 3.55 |
| 8.0 - 811 | | 3.60 |
| 9.0 - 912 | | 3.65 |
| 10.0 - 1013 | | 3.71 |
| 11.0 - 1115 | | 3.76 |
| 12.0 - 1216 | RATED* | 3.81 |
| 13.0 - 1317 | | -- |
| 14.0 - 1419 | | -- |

*Rated Burst Pressure and Stent Rated Burst Pressure. DO NOT EXCEED.

Contents (1)




CL (1) Includes CLIPIT™ Hypotube Clip

GW R 0.014in (≤0.36mm) Recommended Guidewire

GC R 5F (≥0.058in/1.47mm) Recommended Guide Catheter

| | | | |
|---|---|---|---|
| **GTIN** | 08714729370314 | LOT | 12345678 |
| REF Catalog No. | H7493892825350 | Use By | 2010-12-31 |

STERILE EO Sterilized using ethylene oxide.

90244533-01

Internal BSC Bar Code

92425134-45A

CE 0344

**Made in MALAYSIA**
PMT 741, Persiaran Cassia Selatan 1
Taman Perindustrian Batu Kawan
14110 Bandar Cassia,
Pulau Pinang, MALAYSIA

Boston Scientific
Maverick²™
3.5mm x 25mm
GTIN 08714729370314
REF H7493892825350
LOT 12345678

Boston Scientific
Maverick²™
3.5mm x 25mm
GTIN 08714729370314
REF H7493892825350
LOT 12345678

(01)08714729370314(17)101231(10)12345678 GS1

This product may be protected by one or more patents. Patent information can be obtained at http://www.bostonscientific.com/patents

**Label Specification Part Number:92425134-45A**

Boston Scientific

3.75mm x25mm

# Maverick²™

## MONORAIL™


### PTCA Dilatation Catheter

Catéter de dilatación para ACTP, Cathéter de dilatation pour ACTP, PTCA-Dilatationskatheter, Catetere dilatatore per PTCA, PTCA dilatatiekatheter, PTCA拡張カテーテル, PTCA-dilatationskateter, Καθετήρας διαστολής PTCA, Cateter de Dilatação para PTCA, PTCA-dilatationskateter, PTCA-tágítókatéter, Dilatační katétr pro PTCA, Cewnik rozszerzający do PTCA, PTCA-dilatasjonskateter, PTKA Dilatasyon Kateteri

| atm - kPa Pressure | | 3.75mm Balloon O.D. |
|---|---|---|
| 5.0 - 507 | | 3.70 |
| 6.0 - 608 | NOMINAL | 3.75 |
| 7.0 - 709 | | 3.80 |
| 8.0 - 811 | | 3.85 |
| 9.0 - 912 | | 3.90 |
| 10.0 - 1013 | | 3.95 |
| 11.0 - 1115 | | 4.00 |
| 12.0 - 1216 | RATED* | 4.05 |
| 13.0 - 1317 | | -- |
| 14.0 - 1419 | | -- |

*Rated Burst Pressure and Stent Rated Burst Pressure. DO NOT EXCEED.

Contents (1)




CL (1) Includes CLIPIT™ Hypotube Clip

GW R 0.014in (≤0.36mm) Recommended Guidewire

GC R 5F (≥0.058in/1.47mm) Recommended Guide Catheter

| | | | |
|---|---|---|---|
| GTIN | 08714729370321 | LOT | 12345678 |
| REF Catalog No. | H7493892825370 | Use By | 2010-12-31 |

STERILE EO Sterilized using ethylene oxide.

90244533-01

Internal BSC Bar Code

92425134-46A

Boston Scientific
Maverick²™
3.75mm x 25mm
GTIN 08714729370321
REF H7493892825370
LOT 12345678

Boston Scientific
Maverick²™
3.75mm x 25mm
GTIN 08714729370321
REF H7493892825370
LOT 12345678

CE 0344

(01)08714729370321(17)101231(10)12345678 GS1

**Made in MALAYSIA**
PMT 741, Persiaran Cassia Selatan 1
Taman Perindustrian Batu Kawan
14110 Bandar Cassia,
Pulau Pinang, MALAYSIA

This product may be protected by one or more patents. Patent information can be obtained at http://www.bostonscientific.com/patents

**Label Specification Part Number:92425134-46A**

Boston Scientific

**4.0mm x 25mm**

# Maverick²™

## MONORAIL™


### PTCA Dilatation Catheter

Catéter de dilatación para ACTP, Cathéter de dilatation pour ACTP, PTCA-Dilatationskatheter, Catetere dilatatore per PTCA, PTCA dilatatiekatheter, PTCA拡張カテーテル, PTCA-dilatationskateter, Καθετήρας διαστολής PTCA, Cateter de Dilatação para PTCA, PTCA-dilatationskateter, PTCA-tágítókatéter, Dilatační katétr pro PTCA, Cewnik rozszerzający do PTCA, PTCA-dilatasjonskateter, PTKA Dilatasyon Kateteri

| atm - kPa Pressure | | 4.0mm Balloon O.D. |
|---|---|---|
| 5.0 - 507 | | 3.95 |
| 6.0 - 608 | NOMINAL | 4.00 |
| 7.0 - 709 | | 4.05 |
| 8.0 - 811 | | 4.10 |
| 9.0 - 912 | | 4.15 |
| 10.0 - 1013 | | 4.20 |
| 11.0 - 1115 | | 4.25 |
| 12.0 - 1216 | RATED* | 4.31 |
| 13.0 - 1317 | | -- |
| 14.0 - 1419 | | -- |

*Rated Burst Pressure and Stent Rated Burst Pressure. DO NOT EXCEED.

Contents (1)




CL (1) Includes CLIPIT™ Hypotube Clip

GW R 0.014in (≤0.36mm) Recommended Guidewire

GC R 5F (≥0.058in/1.47mm) Recommended Guide Catheter

| | | | |
|---|---|---|---|
| **GTIN** | 08714729370338 | LOT | 12345678 |
| REF Catalog No. | H749389282540o | Use By | 2010-12-31 |

STERILE EO Sterilized using ethylene oxide.

90244533-01

Internal BSC Bar Code

92425134-47A

CE 0344

**Made in MALAYSIA**
PMT 741, Persiaran Cassia Selatan 1
Taman Perindustrian Batu Kawan
14110 Bandar Cassia,
Pulau Pinang, MALAYSIA

Boston Scientific
Maverick²™
4.0mm x 25mm
GTIN 08714729370338
REF H7493892825400
LOT 12345678

Boston Scientific
Maverick²™
4.0mm x 25mm
GTIN 08714729370338
REF H7493892825400
LOT 12345678

(01)08714729370338(17)101231(10)12345678 GS1

This product may be protected by one or more patents. Patent information can be obtained at http://www.bostonscientific.com/patents

**Label Specification Part Number:92425134-47A**

Boston Scientific

**2.0mm x 30mm**

# Maverick²™

## MONORAIL™


### PTCA Dilatation Catheter

Catéter de dilatación para ACTP, Cathéter de dilatation pour ACTP, PTCA-Dilatationskatheter, Catetere dilatatore per PTCA, PTCA dilatatiekatheter, PTCA拡張カテーテル, PTCA-dilatationskateter, Καθετήρας διαστολής PTCA, Cateter de Dilatação para PTCA, PTCA-dilatationskateter, PTCA-tágítókatéter, Dilatační katétr pro PTCA, Cewnik rozszerzający do PTCA, PTCA-dilatasjonskateter, PTKA Dilatasyon Kateteri

| atm - kPa Pressure | | 2.0mm Balloon O.D. |
|---|---|---|
| 5.0 - 507 | | 1.97 |
| 6.0 - 608 | NOMINAL | 2.00 |
| 7.0 - 709 | | 2.03 |
| 8.0 - 811 | | 2.06 |
| 9.0 - 912 | | 2.09 |
| 10.0 - 1013 | | 2.12 |
| 11.0 - 1115 | | 2.15 |
| 12.0 - 1216 | RATED* | 2.19 |
| 13.0 - 1317 | | -- |
| 14.0 - 1419 | | -- |

*Rated Burst Pressure. DO NOT EXCEED.

Contents (1)

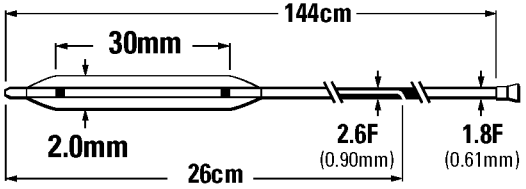


CL (1) Includes CLIPIT™ Hypotube Clip

GW R 0.014in (≤0.36mm) Recommended Guidewire

GC R 5F (≥0.058in/1.47mm) Recommended Guide Catheter

| | | | |
|---|---|---|---|
| **GTIN** | 08714729370345 | LOT | 12345678 |
| REF Catalog No. | H749389283020 0 | Use By | 2010-12-31 |

STERILE EO Sterilized using ethylene oxide.

90244533-01

Internal BSC Bar Code

92425134-48A

CE 0344

**Made in MALAYSIA**
PMT 741, Persiaran Cassia Selatan 1
Taman Perindustrian Batu Kawan
14110 Bandar Cassia,
Pulau Pinang, MALAYSIA

Boston Scientific
Maverick²™
2.0mm x 30mm
GTIN 08714729370345
REF H7493892830200
LOT 12345678

Boston Scientific
Maverick²™
2.0mm x 30mm
GTIN 08714729370345
REF H7493892830200
LOT 12345678

(01)08714729370345(17)101231(10)12345678 GS1

This product may be protected by one or more patents. Patent information can be obtained at http://www.bostonscientific.com/patents

**Label Specification Part Number:92425134-48A**

Boston Scientific

2.25mm x30mm

# Maverick²™

## MONORAIL™


### PTCA Dilatation Catheter

Catéter de dilatación para ACTP, Cathéter de dilatation pour ACTP, PTCA-Dilatationskatheter, Catetere dilatatore per PTCA, PTCA dilatatiekatheter, PTCA拡張カテーテル, PTCA-dilatationskateter, Καθετήρας διαστολής PTCA, Cateter de Dilatação para PTCA, PTCA-dilatationskateter, PTCA-tágítókatéter, Dilatační katétr pro PTCA, Cewnik rozszerzający do PTCA, PTCA-dilatasjonskateter, PTKA Dilatasyon Kateteri

| atm - kPa Pressure | | 2.25mm Balloon O.D. |
|---|---|---|
| 5.0 - 507 | | 2.22 |
| 6.0 - 608 | NOMINAL | 2.25 |
| 7.0 - 709 | | 2.28 |
| 8.0 - 811 | | 2.31 |
| 9.0 - 912 | | 2.35 |
| 10.0 - 1013 | | 2.38 |
| 11.0 - 1115 | | 2.41 |
| 12.0 - 1216 | | 2.44 |
| 13.0 - 1317 | | 2.47 |
| 14.0 - 1419 | RATED* | 2.51 |

*Rated Burst Pressure and Stent Rated Burst Pressure. DO NOT EXCEED.

Contents (1)

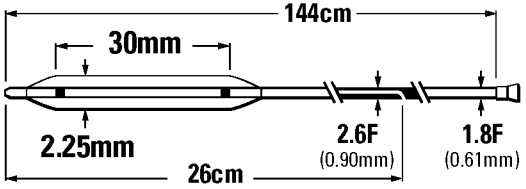


CL (1) Includes CLIPIT™ Hypotube Clip

GW R 0.014in (≤0.36mm) Recommended Guidewire

GC R 5F (≥0.058in/1.47mm) Recommended Guide Catheter

| | | | |
|---|---|---|---|
| GTIN | 08714729370352 | LOT | 12345678 |
| REF Catalog No. | H7493892830220 | Use By | 2010-12-31 |

STERILE EO Sterilized using ethylene oxide.

90244533-01

Internal BSC Bar Code

92425134-49A

Boston Scientific
Maverick²™
2.25mm x 30mm
GTIN 08714729370352
REF H7493892830220
LOT 12345678

Boston Scientific
Maverick²™
2.25mm x 30mm
GTIN 08714729370352
REF H7493892830220
LOT 12345678

CE 0344

(01)08714729370352(17)101231(10)12345678 GS1

**Made in MALAYSIA**
PMT 741, Persiaran Cassia Selatan 1
Taman Perindustrian Batu Kawan
14110 Bandar Cassia,
Pulau Pinang, MALAYSIA

This product may be protected by one or more patents. Patent information can be obtained at http://www.bostonscientific.com/patents

**Label Specification Part Number:92425134-49A**

Boston Scientific

2.5mm x30mm

# Maverick²™

## MONORAIL™


### PTCA Dilatation Catheter

Catéter de dilatación para ACTP, Cathéter de dilatation pour ACTP, PTCA-Dilatationskatheter, Catetere dilatatore per PTCA, PTCA dilatatiekatheter, PTCA拡張カテーテル, PTCA-dilatationskateter, Καθετήρας διαστολής PTCA, Cateter de Dilatação para PTCA, PTCA-dilatationskateter, PTCA-tágítókatéter, Dilatační katétr pro PTCA, Cewnik rozszerzający do PTCA, PTCA-dilatasjonskateter, PTKA Dilatasyon Kateteri

| atm - kPa Pressure | | 2.5mm Balloon O.D. |
|---|---|---|
| 5.0 - 507 | | 2.46 |
| 6.0 - 608 | NOMINAL | 2.50 |
| 7.0 - 709 | | 2.54 |
| 8.0 - 811 | | 2.58 |
| 9.0 - 912 | | 2.62 |
| 10.0 - 1013 | | 2.67 |
| 11.0 - 1115 | | 2.71 |
| 12.0 - 1216 | | 2.75 |
| 13.0 - 1317 | | 2.79 |
| 14.0 - 1419 | RATED* | 2.83 |

*Rated Burst Pressure and Stent Rated Burst Pressure. DO NOT EXCEED.

Contents (1)

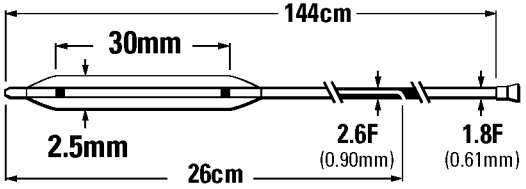


CL (1) Includes CLIPIT™ Hypotube Clip

GW R 0.014in (≤0.36mm) Recommended Guidewire

GC R 5F (≥0.058in/1.47mm) Recommended Guide Catheter

| | | | |
|---|---|---|---|
| GTIN | 08714729370369 | LOT | 12345678 |
| REF Catalog No. | H7493892830250 | Use By | 2010-12-31 |

STERILE EO Sterilized using ethylene oxide.

90244533-01

Internal BSC Bar Code

92425134-50A

Boston Scientific
Maverick²™
2.5mm x 30mm
GTIN 08714729370369
REF H7493892830250
LOT 12345678

Boston Scientific
Maverick²™
2.5mm x 30mm
GTIN 08714729370369
REF H7493892830250
LOT 12345678

CE 0344

(01)08714729370369(17)101231(10)12345678 GS1

**Made in MALAYSIA**
PMT 741, Persiaran Cassia Selatan 1
Taman Perindustrian Batu Kawan
14110 Bandar Cassia,
Pulau Pinang, MALAYSIA

This product may be protected by one or more patents. Patent information can be obtained at http://www.bostonscientific.com/patents

**Label Specification Part Number:92425134-50A**

Boston Scientific

**2.75mm x30mm**

# Maverick²™

## MONORAIL™


### PTCA Dilatation Catheter

Catéter de dilatación para ACTP, Cathéter de dilatation pour ACTP, PTCA-Dilatationskatheter, Catetere dilatatore per PTCA, PTCA dilatatiekatheter, PTCA拡張カテーテル, PTCA-dilatationskateter, Καθετήρας διαστολής PTCA, Cateter de Dilatação para PTCA, PTCA-dilatationskateter, PTCA-tágítókatéter, Dilatační katétr pro PTCA, Cewnik rozszerzający do PTCA, PTCA-dilatasjonskateter, PTKA Dilatasyon Kateteri

| atm - kPa Pressure | | 2.75mm Balloon O.D. |
|---|---|---|
| 5.0 - 507 | | 2.71 |
| 6.0 - 608 | NOMINAL | 2.75 |
| 7.0 - 709 | | 2.79 |
| 8.0 - 811 | | 2.83 |
| 9.0 - 912 | | 2.87 |
| 10.0 - 1013 | | 2.91 |
| 11.0 - 1115 | | 2.95 |
| 12.0 - 1216 | | 2.99 |
| 13.0 - 1317 | | 3.03 |
| 14.0 - 1419 | RATED* | 3.07 |

*Rated Burst Pressure and Stent Rated Burst Pressure. DO NOT EXCEED.

Contents (1)

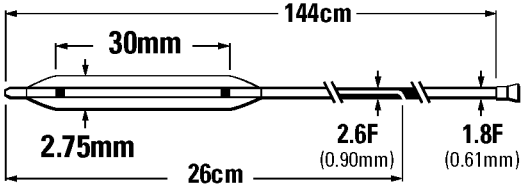


CL (1) Includes CLIPIT™ Hypotube Clip

GW R 0.014in (≤0.36mm) Recommended Guidewire

GC R 5F (≥0.058in/1.47mm) Recommended Guide Catheter

| | | | |
|---|---|---|---|
| **GTIN** | 08714729370376 | LOT | 12345678 |
| REF Catalog No. | H749389283027o | Use By | 2010-12-31 |

STERILE EO Sterilized using ethylene oxide.

90244533-01

Internal BSC Bar Code

92425134-51A

CE 0344

**Made in MALAYSIA**
PMT 741, Persiaran Cassia Selatan 1
Taman Perindustrian Batu Kawan
14110 Bandar Cassia,
Pulau Pinang, MALAYSIA

Boston Scientific
Maverick²™
2.75mm x 30mm
GTIN 08714729370376
REF H7493892830270
LOT 12345678

Boston Scientific
Maverick²™
2.75mm x 30mm
GTIN 08714729370376
REF H7493892830270
LOT 12345678

(01)08714729370376(17)101231(10)12345678 GS1

This product may be protected by one or more patents. Patent information can be obtained at http://www.bostonscientific.com/patents

**Label Specification Part Number:92425134-51A**

Boston Scientific

**3.0mm x 30mm**

# Maverick²™

## MONORAIL™


### PTCA Dilatation Catheter

Catéter de dilatación para ACTP, Cathéter de dilatation pour ACTP, PTCA-Dilatationskatheter, Catetere dilatatore per PTCA, PTCA dilatatiekatheter, PTCA拡張カテーテル, PTCA-dilatationskateter, Καθετήρας διαστολής PTCA, Cateter de Dilatação para PTCA, PTCA-dilatationskateter, PTCA-tágítókatéter, Dilatační katétr pro PTCA, Cewnik rozszerzający do PTCA, PTCA-dilatasjonskateter, PTKA Dilatasyon Kateteri

| atm - kPa Pressure | | 3.0mm Balloon O.D. |
|---|---|---|
| 5.0 - 507 | | 2.95 |
| 6.0 - 608 | NOMINAL | 3.00 |
| 7.0 - 709 | | 3.05 |
| 8.0 - 811 | | 3.09 |
| 9.0 - 912 | | 3.14 |
| 10.0 - 1013 | | 3.18 |
| 11.0 - 1115 | | 3.23 |
| 12.0 - 1216 | | 3.28 |
| 13.0 - 1317 | | 3.32 |
| 14.0 - 1419 | RATED* | 3.37 |

*Rated Burst Pressure and Stent Rated Burst Pressure. DO NOT EXCEED.

Contents (1)

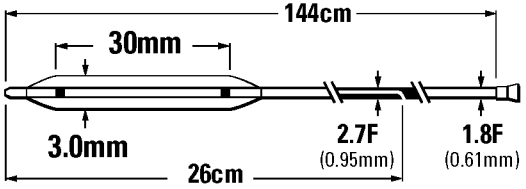


CL (1) Includes CLIPIT™ Hypotube Clip

GW R 0.014in (≤0.36mm) Recommended Guidewire

GC R 5F (≥0.058in/1.47mm) Recommended Guide Catheter

| | | | |
|---|---|---|---|
| **GTIN** | 08714729370383 | LOT | 12345678 |
| REF Catalog No. | H749389283030 0 | Use By | 2010-12-31 |

STERILE EO Sterilized using ethylene oxide.

90244533-01

Internal BSC Bar Code

92425134-52A

CE 0344

**Made in MALAYSIA**
PMT 741, Persiaran Cassia Selatan 1
Taman Perindustrian Batu Kawan
14110 Bandar Cassia,
Pulau Pinang, MALAYSIA

Boston Scientific
Maverick²™
3.0mm x 30mm
GTIN 08714729370383
REF H7493892830300
LOT 12345678

Boston Scientific
Maverick²™
3.0mm x 30mm
GTIN 08714729370383
REF H7493892830300
LOT 12345678

(01)08714729370383(17)101231(10)12345678 GS1

This product may be protected by one or more patents. Patent information can be obtained at http://www.bostonscientific.com/patents

**Label Specification Part Number:92425134-52A**

Boston Scientific

3.25mm x30mm

# Maverick²™

## MONORAIL™


### PTCA Dilatation Catheter

Catéter de dilatación para ACTP, Cathéter de dilatation pour ACTP, PTCA-Dilatationskatheter, Catetere dilatatore per PTCA, PTCA dilatatiekatheter, PTCA拡張カテーテル, PTCA-dilatationskateter, Καθετήρας διαστολής PTCA, Cateter de Dilatação para PTCA, PTCA-dilatationskateter, PTCA-tágítókatéter, Dilatační katétr pro PTCA, Cewnik rozszerzający do PTCA, PTCA-dilatasjonskateter, PTKA Dilatasyon Kateteri

| atm - kPa Pressure | | 3.25mm Balloon O.D. |
|---|---|---|
| 5.0 - 507 | | 3.20 |
| 6.0 - 608 | NOMINAL | 3.25 |
| 7.0 - 709 | | 3.30 |
| 8.0 - 811 | | 3.34 |
| 9.0 - 912 | | 3.39 |
| 10.0 - 1013 | | 3.43 |
| 11.0 - 1115 | | 3.48 |
| 12.0 - 1216 | | 3.52 |
| 13.0 - 1317 | | 3.57 |
| 14.0 - 1419 | RATED* | 3.61 |

*Rated Burst Pressure and Stent Rated Burst Pressure. DO NOT EXCEED.

Contents (1)

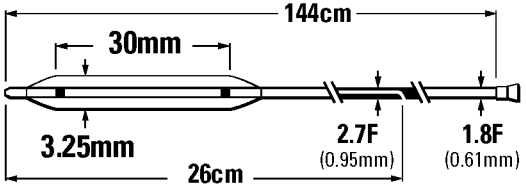


CL (1) Includes CLIPIT™ Hypotube Clip

GW R 0.014in (≤0.36mm) Recommended Guidewire

GC R 5F (≥0.058in/1.47mm) Recommended Guide Catheter

| | | | |
|---|---|---|---|
| **GTIN** | 08714729370390 | LOT | 12345678 |
| REF Catalog No. | H749389283032o | Use By | 2010-12-31 |

STERILE EO Sterilized using ethylene oxide.

90244533-01

Internal BSC Bar Code

92425134-53A

CE 0344

**Made in MALAYSIA**
PMT 741, Persiaran Cassia Selatan 1
Taman Perindustrian Batu Kawan
14110 Bandar Cassia,
Pulau Pinang, MALAYSIA

Boston Scientific
Maverick²™
3.25mm x 30mm
GTIN 08714729370390
REF H7493892830320
LOT 12345678

Boston Scientific
Maverick²™
3.25mm x 30mm
GTIN 08714729370390
REF H7493892830320
LOT 12345678

(01)08714729370390(17)101231(10)12345678 GS1

This product may be protected by one or more patents. Patent information can be obtained at http://www.bostonscientific.com/patents

**Label Specification Part Number:92425134-53A**

Boston Scientific

3.5mm x30mm

# Maverick²™

## MONORAIL™


### PTCA Dilatation Catheter

Catéter de dilatación para ACTP, Cathéter de dilatation pour ACTP, PTCA-Dilatationskatheter, Catetere dilatatore per PTCA, PTCA dilatatiekatheter, PTCA拡張カテーテル, PTCA-dilatationskateter, Καθετήρας διαστολής PTCA, Cateter de Dilatação para PTCA, PTCA-dilatationskateter, PTCA-tágítókatéter, Dilatační katétr pro PTCA, Cewnik rozszerzający do PTCA, PTCA-dilatasjonskateter, PTKA Dilatasyon Kateteri

| atm - kPa Pressure | | 3.5mm Balloon O.D. |
|---|---|---|
| 5.0 - 507 | | 3.45 |
| 6.0 - 608 | NOMINAL | 3.50 |
| 7.0 - 709 | | 3.55 |
| 8.0 - 811 | | 3.60 |
| 9.0 - 912 | | 3.65 |
| 10.0 - 1013 | | 3.71 |
| 11.0 - 1115 | | 3.76 |
| 12.0 - 1216 | RATED* | 3.81 |
| 13.0 - 1317 | | -- |
| 14.0 - 1419 | | -- |

*Rated Burst Pressure and Stent Rated Burst Pressure. DO NOT EXCEED.

Contents (1)

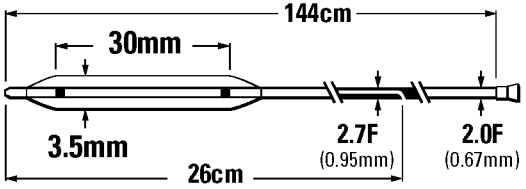


CL (1) Includes CLIPIT™ Hypotube Clip

GW R 0.014in (≤0.36mm) Recommended Guidewire

GC R 5F (≥0.058in/1.47mm) Recommended Guide Catheter

| | | | |
|---|---|---|---|
| GTIN | 08714729370406 | LOT | 12345678 |
| REF Catalog No. | H749389283035O | Use By | 2010-12-31 |

STERILE EO Sterilized using ethylene oxide.

90244533-01

Internal BSC Bar Code

92425134-54A

CE 0344

Made in MALAYSIA
PMT 741, Persiaran Cassia Selatan 1
Taman Perindustrian Batu Kawan
14110 Bandar Cassia,
Pulau Pinang, MALAYSIA

Boston Scientific
Maverick²™
3.5mm x 30mm
GTIN 08714729370406
REF H7493892830350
LOT 12345678

Boston Scientific
Maverick²™
3.5mm x 30mm
GTIN 08714729370406
REF H7493892830350
LOT 12345678

(01)08714729370406(17)101231(10)12345678 GS1

This product may be protected by one or more patents. Patent information can be obtained at http://www.bostonscientific.com/patents

**Label Specification Part Number:92425134-54A**

Boston Scientific

3.75mm x30mm

# Maverick²™

## MONORAIL™


### PTCA Dilatation Catheter

Catéter de dilatación para ACTP, Cathéter de dilatation pour ACTP, PTCA-Dilatationskatheter, Catetere dilatatore per PTCA, PTCA dilatatiekatheter, PTCA拡張カテーテル, PTCA-dilatationskateter, Καθετήρας διαστολής PTCA, Cateter de Dilatação para PTCA, PTCA-dilatationskateter, PTCA-tágítókatéter, Dilatační katétr pro PTCA, Cewnik rozszerzający do PTCA, PTCA-dilatasjonskateter, PTKA Dilatasyon Kateteri

| atm - kPa Pressure | | 3.75mm Balloon O.D. |
|---|---|---|
| 5.0 - 507 | | 3.70 |
| 6.0 - 608 | NOMINAL | 3.75 |
| 7.0 - 709 | | 3.80 |
| 8.0 - 811 | | 3.85 |
| 9.0 - 912 | | 3.90 |
| 10.0 - 1013 | | 3.95 |
| 11.0 - 1115 | | 4.00 |
| 12.0 - 1216 | RATED* | 4.05 |
| 13.0 - 1317 | | -- |
| 14.0 - 1419 | | -- |

*Rated Burst Pressure and Stent Rated Burst Pressure. DO NOT EXCEED.

Contents (1)

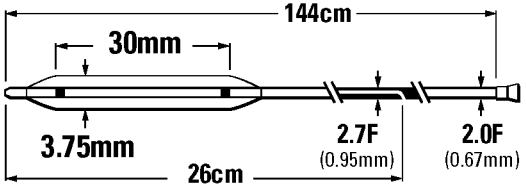


CL (1) Includes CLIPIT™ Hypotube Clip

GW R 0.014in (≤0.36mm) Recommended Guidewire

GC R 5F (≥0.058in/1.47mm) Recommended Guide Catheter

| | | | |
|---|---|---|---|
| GTIN | 08714729370413 | LOT | 12345678 |
| REF Catalog No. | H7493892830370 | Use By | 2010-12-31 |

STERILE EO Sterilized using ethylene oxide.

90244533-01

Internal BSC Bar Code

92425134-55A

CE 0344

Made in MALAYSIA
PMT 741, Persiaran Cassia Selatan 1
Taman Perindustrian Batu Kawan
14110 Bandar Cassia,
Pulau Pinang, MALAYSIA

Boston Scientific
Maverick²™
3.75mm x 30mm
GTIN 08714729370413
REF H7493892830370
LOT 12345678

Boston Scientific
Maverick²™
3.75mm x 30mm
GTIN 08714729370413
REF H7493892830370
LOT 12345678

(01)08714729370413(17)101231(10)12345678 GS1

This product may be protected by one or more patents. Patent information can be obtained at http://www.bostonscientific.com/patents

**Label Specification Part Number:92425134-55A**

Boston Scientific

**4.0mm x 30mm**

# Maverick²™

## MONORAIL™


### PTCA Dilatation Catheter

Catéter de dilatación para ACTP, Cathéter de dilatation pour ACTP, PTCA-Dilatationskatheter, Catetere dilatatore per PTCA, PTCA dilatatiekatheter, PTCA拡張カテーテル, PTCA-dilatationskateter, Καθετήρας διαστολής PTCA, Cateter de Dilatação para PTCA, PTCA-dilatationskateter, PTCA-tágítókatéter, Dilatační katétr pro PTCA, Cewnik rozszerzający do PTCA, PTCA-dilatasjonskateter, PTKA Dilatasyon Kateteri

| atm - kPa Pressure | | 4.0mm Balloon O.D. |
|---|---|---|
| 5.0 - 507 | | 3.95 |
| 6.0 - 608 | NOMINAL | 4.00 |
| 7.0 - 709 | | 4.05 |
| 8.0 - 811 | | 4.10 |
| 9.0 - 912 | | 4.15 |
| 10.0 - 1013 | | 4.20 |
| 11.0 - 1115 | | 4.25 |
| 12.0 - 1216 | RATED* | 4.31 |
| 13.0 - 1317 | | -- |
| 14.0 - 1419 | | -- |

*Rated Burst Pressure and Stent Rated Burst Pressure. DO NOT EXCEED.

Contents (1)

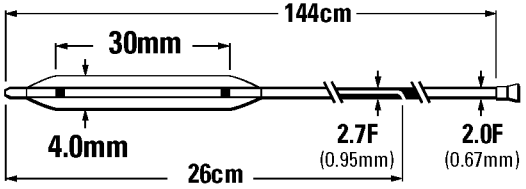


CL (1) Includes CLIPIT™ Hypotube Clip

GW R 0.014in (≤0.36mm) Recommended Guidewire

GC R 5F (≥0.058in/1.47mm) Recommended Guide Catheter

| | | | |
|---|---|---|---|
| **GTIN** | 08714729370420 | LOT | 12345678 |
| REF Catalog No. | H749389283040o | Use By | 2010-12-31 |

STERILE EO Sterilized using ethylene oxide.

90244533-01

Internal BSC Bar Code

92425134-56A

CE 0344

**Made in MALAYSIA**
PMT 741, Persiaran Cassia Selatan 1
Taman Perindustrian Batu Kawan
14110 Bandar Cassia,
Pulau Pinang, MALAYSIA

Boston Scientific
Maverick²™
4.0mm x 30mm
GTIN 08714729370420
REF H7493892830400
LOT 12345678

Boston Scientific
Maverick²™
4.0mm x 30mm
GTIN 08714729370420
REF H7493892830400
LOT 12345678

(01)08714729370420(17)101231(10)12345678 GS1

This product may be protected by one or more patents. Patent information can be obtained at http://www.bostonscientific.com/patents

**Label Specification Part Number:92425134-56A**