
AOZ

CERTIFICATE OF ANALYSIS

Doc. No:	5091AOZ-CA V16
Batch No:	250551
Code:	5091AOZ
Exp. Date:	12-2026

This certificate relates to the above specified product batch and number only. The product has been tested according to our standard quality control program. The product is guaranteed when stored according to the instruction in the manual till the indicated expiry date.

Components:	**Lot No:**	**Exp. Date:**
Microtiter plate	250468	12-2026
Conjugate	250469	12-2026
Standards 1 - 0,4 - 0,16 - 0,064 - 0,0256 - 0,01 - 0 ng/ml	250470	02-2028
Standaard 100 ng/ml	250471	02-2028
Sample Dilution buffer	250462	06-2027
Dilution buffer	250188	03-2027
Rinsing buffer	250333	04-2027
TMB substrate	241194	07-2028
Stop solution	250185	03-2027
Protocol	Code 5091AOZ [12]02.24	

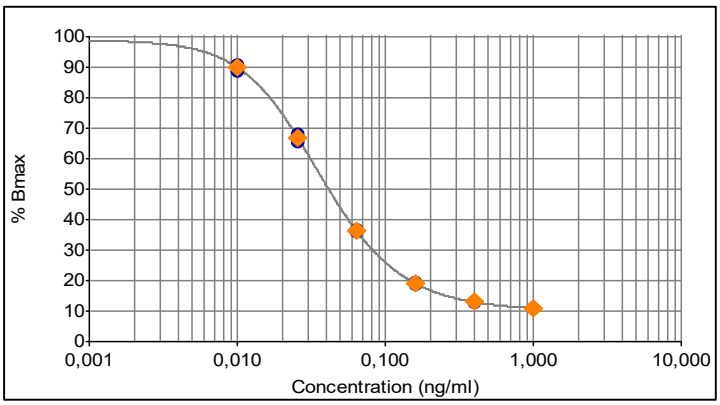

Validation criteria

Bmax > 0.8 OD.
Blank < 0.2 OD.

Concentration (ng/ml)	Accepted Range %Bmax	Mean %Bmax
STD 0,4	13 - 25	13
STD 0,16	17 - 30	19
STD 0,064	28 - 40	36
STD 0,0256	56 - 72	67

Performed by: TK date: 07-07-2025

Accepted by:

ISO 9001 BUREAU VERITAS Certification

This product is produced under the control of a management system approved by Bureau Veritas certification in accordance with the standard ISO 9001: 2015 Bureau Veritas Certification N°3089368