KLEOS
medical education from smith&nephew

Bone&JointScience
Our Innovation in Focus

Vol 03, No 02 - January 2012

The Utilization of Electromagnetic Tracking to Facilitate Distal Targeting During Intramedullary Nailing

Chris Moore MS[1], Charles Heotis BE[1], Nick Ritchey BSME[1]

1 Smith & Nephew, Inc., Memphis, TN, USA

Summary

Locked intramedullary (IM) nailing may be considered the standard treatment for long-bone shaft fractures. While this technique has been shown to reduce malunion and limb shortening risk, locking the nail into place is a very challenging step of the procedure. Several technologies have been introduced to help facilitate accurate screw insertion and locking. However, electromagnetic (EM) tracking has emerged as perhaps the most promising alternative. The SURESHOT® Distal Targeting System (Smith & Nephew, Inc., Memphis, TN, USA) represents an innovative application of EM technology. Utilizing an ionizing radiation free EM field, this system is capable of accurately mapping the position and orientation of a sensor that is positioned within the IM nail. Data obtained from this sensor enables the system to display a virtual representation of the nail and screw insertion path. Using real-time virtual feedback, the surgeon simply achieves the desired alignment and completes distal targeting and locking. SURESHOT may support improved outcomes in fracture patients by significantly improving drilling accuracy, reducing locking time and minimizing requisite radiation exposure in the operating room. Research is currently underway to further explore the clinical efficacy of this system.

Introduction

Intramedullary (IM) nailing and fixation has emerged as a standard treatment for frequently encountered long-bone shaft fractures [1, 2]. As with most orthopaedic procedures, an evolving surgical technique has helped to greatly improve clinical outcomes in fracture patients. A key development in IM nailing was the inclusion of locking screws in the proximal and distal portions of the nail. Locking the nail into place helps to control limb length, rotation, and angulation, which reduces malunion and shortening risk [1]. This technique also enables the treatment of difficult proximal, distal, and unstable shaft fractures [3]. While the benefits of IM nail locking are not in question, there remains one key consideration. Locking may be considered the most difficult step of this procedure [2].

Before the IM nail can be locked into position, the screw entry point and insertion path must be accurately determined [2].

Traditionally, this step has required the use of intraoperative x-ray. A C-Arm fluoroscopy unit allows the surgeon to obtain a radiographic image of the nail in vivo. Insertion of the screw is then attempted utilizing a freehand drilling technique. While common, this approach is technically demanding and requires considerable experience to effectively be executed [2]. Furthermore, the need to repeatedly adjust C-Arm orientation and the screw insertion path can extend operative time and increase the duration of x-ray exposure for both the patient and operating room staff [4, 5]. With just one additional minute of C-Arm use, radiation exposure can increase by approximately 0.4-4.0 rad [6, 7]. Therefore, improving first-time drilling and targeting accuracy during locking is critical.

Alternative targeting technologies have been introduced to improve the accuracy and ease of IM nail locking. Mechanical and robotic guidance have both been utilized with some success [2, 8-10]. Here, radiographic imaging and opaque markers allow the surgical space to be effectively mapped. Once nail position and orientation are determined, the screw insertion path is mechanically maintained by an encompassing structure until locking is complete. However, there are two key limitations with this approach. First, nail geometry commonly changes during insertion, creating the risk of positioning error [11]. Second, a fixed mechanical path and enclosed surgical space may be considered cumbersome and obtrusive to the surgeon [2]. A more ideal system would provide accurate guidance, while preserving operative freedom of movement and patient access during the duration of the procedure.


Computerized optical tracking systems have been successfully utilized in the clinical environment due to their high degree of accuracy [12-15]. Once the coordinates of the surgical space, patient, and instrumentation are all established, a camera and computer interface can be used to provide real-time virtual feedback to the surgeon [2, 13]. While this system would indeed seem far more ideal, the technology is critically limited during IM nailing. All optical systems require a direct line of sight between the camera and light-emitting sensor [13, 15]. This is simply not possible when the surgical target is embedded within the patient's body [13, 15]. Fortunately, an alternative computerized tracking technology does appear to be particularly well suited for this application. Specifically, electromagnetic tracking systems (EMS) appear to support accurate, rapid, and reliable locking results during IM fracture fixation.

Electromagnetic Tracking

EMS systems are designed to determine the position and orientation of special sensors that have been positioned within surgical tools. Tracking begins with a computerized control unit that powers and controls an electromagnetic (EM) field generator. The generator projects a safe EM field across the operative site, which is free of potentially dangerous ionizing radiation [16]. It is this field that enables a highly precise map to be drawn of the surgical space. When the surgical tool containing the system sensor is placed into that mapped space, the sensor emits a small electric current. Once that current is converted to a digital signal, the control unit can identify the tool and plot its exact location. That data is then sent to a host computer which can display the tracking information via application software. Unlike optical tracking systems that are limited by line of sight, EM tracking can be accurately performed while the sensor is contained within the body.

There are several key features that make EMS particularly well suited for utilization during IM nailing [15]. First and foremost, EM tracking can precisely track surgical instruments, independent of line of sight [13, 15]. This is made possible by the EM field. Within the surgical space map, all coordinates can be measured around a directional Z-axis (Figure 1A). The key to tracking is that the system sensor positioned within the surgical tool is also oriented around its own Z-axis (Figure 1B). This is what allows the control unit to assess the sensors' relative position and orientation within the mapped space. A second key feature of EMS is the refresh rate. Sensor data must be obtained and processed by the control unit fast enough to ensure real-time virtual feedback to the surgeon. As compared to other tracking systems, EMS does support a refresh rate that is acceptable for surgical use [13, 15]. Finally, EMS is highly conducive to the trauma operating room environment. In contrast to mechanical and robotic guidance systems, EMS is very unobtrusive and does not restrict or alter surgeon access to the patient [2, 15]. Furthermore, EMS is not adversely affected by light and sound levels within the operating room, and is not overly susceptible to field deviation when exposed to conductive or ferromagnetic objects [13, 17]. Any potential for EM field interference is mitigated by the relatively small distance between the system sensor and the field generator [18]. Further, it is important to account for any metallic items that may still be in the field, including any instruments or metal structures that may be supporting the operative limb.


Figure 1: The coordinate system of the generated EM field (A), and the Z-axis orientation within the length of the sensor coil (B)

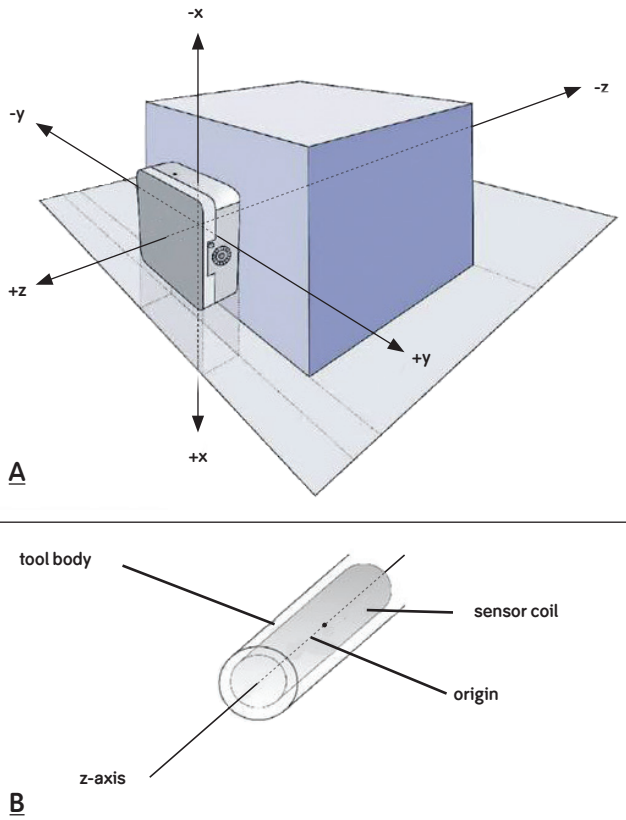

The Application of EMS during Distal Locking

The SURESHOT® Distal Targeting System (Smith & Nephew, Inc., Memphis, TN, USA) represents an innovative application of EMS technology. All of the essential tracking elements are contained within this system. However, the design of SURESHOT has been adapted specifically to facilitate distal locking during IM nailing. The computerized control unit is contained within the SURESHOT display and interface unit, while the EM field generator is actually located within the hand-held targeting device (Figure 2). The targeter is capable of projecting a focused EM field across the surgical site, similar to the illumination from a flashlight. Furthermore, the targeter is designed to be held securely and comfortably by the surgeon while distal targeting and locking is completed.


Figure 2: The SURESHOT Distal Targeting System (Smith & Nephew, Inc., Memphis, TN, USA)

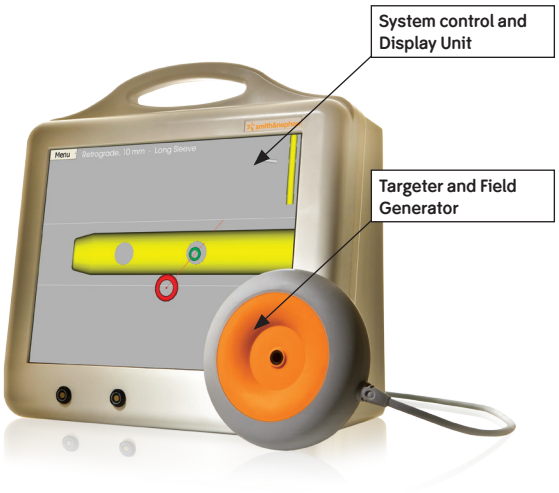

As discussed previously, EMS tracking is made possible by sensor interaction with the projected EM field. With SURESHOT, the sensor and accompanying hardware are designed to perfectly accommodate the TRIGEN® Intramedullary Nail (Smith & Nephew, Inc., Memphis, TN, USA; Figure 3). Once the TRIGEN nail is inserted into the patient, the system is able to reproduce an accurate virtual representation of the nail on the SURESHOT display unit. With the drill bit inserted through the targeter, the surgeon simply aligns the target with the real-time insertion path (the red and green circles illustrated in Figure 2), completes drilling, and then simply inserts the locking screw.

Tornetta et al [19] have verified the accuracy of SURESHOT in the clinical setting. The authors reported first-time locking accuracy for 24 tibial and femoral shaft fracture cases. Drilling accuracy of 100% and 96% was observed for each fracture type, respectively. Moreover, when compared to the standard freehand and guidance free technique, SURESHOT was found to reduce locking time by 32-48%. The authors note that these savings could reduce the time of C-Arm use by approximately 36-49 seconds, which is equivalent to approximately 0.785-2.362 rad of radiation emission [19]. While these results are both impressive and encouraging, it is not yet clear how this improved locking precision affects the clinical outcome of

Figure 3: System sensor inserted into TRIGEN® Intramedullary Nail (Smith & Nephew, Inc., Memphis, TN, USA; A), and the clinical application of SURESHOT during distal locking (B)

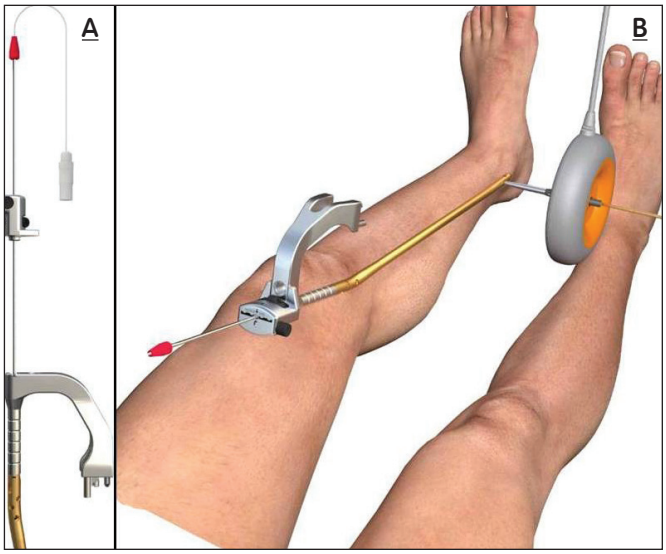

fracture patients. Furthermore, these reductions in radiation exposure have yet to be directly quantified. Smith & Nephew is therefore conducting a prospective, multicenter study to fully assess the clinical efficacy of the SURESHOT system (ClinicalTrials.gov Identifier: NCT01327508).

References

1. **Keast-Butler O, Lutz MJ, Angelini M, Lash N, Pearce D, Crookshank M, Zdero R, Schemitsch EH.** Computer navigation in the reduction and fixation of femoral shaft fractures: A randomized control study. Injury, 2011
2. **Lei H, Sheng L, Manyi W, Junqiang W, Wenyong L.** A biplanar robot navigation system for the distal locking of intramedullary nails. Int J Med Robot 6(1): 61, 2010
3. **Kempf I, Grosse A, Beck G.** Closed locked intramedullary nailing. Its application to comminuted fractures of the femur. J Bone Joint Surg Am 67(5): 709, 1985
4. **Levin PE, Schoen RW, Jr., Browner BD.** Radiation exposure to the surgeon during closed interlocking intramedullary nailing. J Bone Joint Surg Am 69(5): 761, 1987
5. **Sugarman ID, Adam I, Bunker TD.** Radiation dosage during AO locking femoral nailing. Injury 19(5): 336, 1988
6. **Singer G.** Occupational radiation exposure to the surgeon. J Am Acad Orthop Surg 13(1): 69, 2005
7. **Tomei F, Papaleo B, Fantini S, Iavicoli S, Baccolo TP, Rosati MV.** Vascular effects of occupational exposure to low-dose ionizing radiation. Am J Ind Med 30(1): 72, 1996
8. **Wang T, Liu W, Hu L.** BPOR: a fluoroscopy-based robot navigating system for distal locking of intramedullary nails. In Conference on Intelligent Robots and Systems (IROS) Sendia, Japan 2004
9. **Karachalios T, Babis G, Tsarouchas J, Sapkas G, Pantazopoulos T.** The clinical performance of a small diameter tibial nailing system with a mechanical distal aiming device. Injury 31(6): 451, 2000
10. **Krettek C, Konemann B, Miclau T, Kolbli R, Machreich T, Tscherne H.** A mechanical distal aiming device for distal locking in femoral nails. Clin Orthop Relat Res (364): 267, 1999
11. **Arlettaz Y, Akiki A, Chevalley F, Leyvraz PF.** Targeting device for intramedullary nails: a new high-stable mechanical guide. Injury 39(2): 170, 2008
12. **Birkfellner W, Watzinger F, Wanschitz F, Ewers R, Bergmann H.** Calibration of tracking systems in a surgical environment. IEEE Trans Med Imaging 17(5): 737, 1998
13. **Hummel J, Figl M, Kollmann C, Bergmann H, Birkfellner W.** Evaluation of a miniature electromagnetic position tracker. Med Phys 29(10): 2205, 2002
14. **Metson RB, Cosenza MJ, Cunningham MJ, Randolph GW.** Physician experience with an optical image guidance system for sinus surgery. Laryngoscope 110(6): 972, 2000
15. **Yaniv Z, Wilson E, Lindisch D, Cleary K.** Electromagnetic tracking in the clinical environment. Med Phys 36(3): 876, 2009
16. **Moore C, Heeckt P.** Reducing Radiation Risk in Orthopaedic Trauma Surgery. Bone&Joint Science (www.KLEOS.md) 2(7), 2011
17. **Birkfellner W, Watzinger F, Wanschitz F, Enislidis G, Kollmann C, Rafolt D, Nowotny R, Ewers R, Bergmann H.** Systematic distortions in magnetic position digitizers. Med Phys 25(11): 2242, 1998
18. Aurora User Manual - Revision 1.0. Northern Digitial Inc (More information available at: http://www.ndigital.com/medical/aurora.php), 2005
19. **Tornetta P, Patel P, Tseng S, Whitten A, Ricci W.** Distal locking using an electromagnetic field guided computer based real time system. Orthopaedic Trauma Association (OTA) Annual Meeting Poster No. 98, 2009

Great care has been taken to maintain the accuracy of the information contained in the publication. However, neither KLEOS, nor the authors can be held responsible for errors or any consequences arising from the use of the information contained in this publication. The statements or opinions contained in editorials and articles in this journal are solely those of the authors thereof and not of KLEOS. The products, procedures, and therapies described are only to be applied by certified and trained medical professionals in environments specially designed for such procedures. No suggested test or procedure should be carried out unless, in the reader's professional judgment, its risk is justified. Because of rapid advances in the medical sciences, we recommend that independent verification of diagnosis, drugs dosages, and operating methods should be made before any action is taken. Although all advertising material is expected to conform to ethical (medical) standards, inclusion in this publication does not constitute a guarantee or endorsement of the quality or value of such product or of the claims made of it by its manufacturer. Some of the products, names, instruments, treatments, logos, designs, etc. referred to in this journal are also protected by patents and trademarks or by other intellectual property protection laws even though specific reference to this fact is not always made in the text. Therefore, the appearance of a name, instrument, etc. without designation as proprietary is not to be construed as a representation by the publisher that it is in the public domain. This publication, including all parts thereof, is legally protected by copyright. Any use, exploitation or commercialization outside the narrow limits of copyrights legislation, without the publisher's consent, is illegal and liable to prosecution. This applies in particular to photostat reproduction, copying, scanning or duplication of any kind, translating, preparation of microfilms and electronic data processing and storage. Institutions' subscriptions allow to reproduce tables of content or prepare lists of articles including abstracts for internal circulation within the institutions concerned. Permission of the publisher is required for resale or distribution outside the institutions. Permission of the publisher is required for all other derivative works, including compilations and translations. Permission of the publisher is required to store or use electronically any material contained in this journal, including any article or part of an article. For inquiries contact the publisher at the address indicated.

US: Lit.No: 71182126 REV0 01/12

Produced by the Research and Clinical Departments,
Smith & Nephew Inc.
Published by KLEOS, the medical education service
from Smith & Nephew

Published January 2012
Copyright © 2012 by Smith & Nephew Orthopaedics AG
KLEOS, Oberneuhofstrasse 10d, 6340 Baar, Switzerland
Phone +41 41 766 22 55
kleos@smith-nephew.com

Bone&JointScience is available on the KLEOS website,
www.kleos.md, within "Literature"

®Trademark of Smith & Nephew. Reg. US Pat. & TM Off.